



OFFICE OF STATEWIDE HEALTH PLANNING AND DEVELOPMENT
FACILITIES DEVELOPMENT DIVISION

APPLICATION FOR OSHPD PREAPPROVAL OF MANUFACTURER'S CERTIFICATION (OPM)

OFFICE USE ONLY
APPLICATION #: OPM-0094-13

OSHPD Preapproval of Manufacturer's Certification (OPM)


Type: [X] New [ ] Renewal [X] Update to Pre-CBC 2013 OPA Number: OPA-2096-07

Manufacturer Information

Manufacturer: Ortho Clinical Diagnostics Part of the Johnson & Johnson Family of Companies
Manufacturer's Technical Representative: Frank Koetter
Mailing Address: 100 Indigo Creek Drive, MC00891, Rochester, NY 14626-5101
Telephone: 1-585-453-4003 Email: FKoetter@its.jnj.com

Product Information

Product Name: Vitros 3600 Immunodiagnostic System
Product Type: Immunoassay System
Product Model Number: Vitros 3600
General Description: Immune System Blood Analyzer

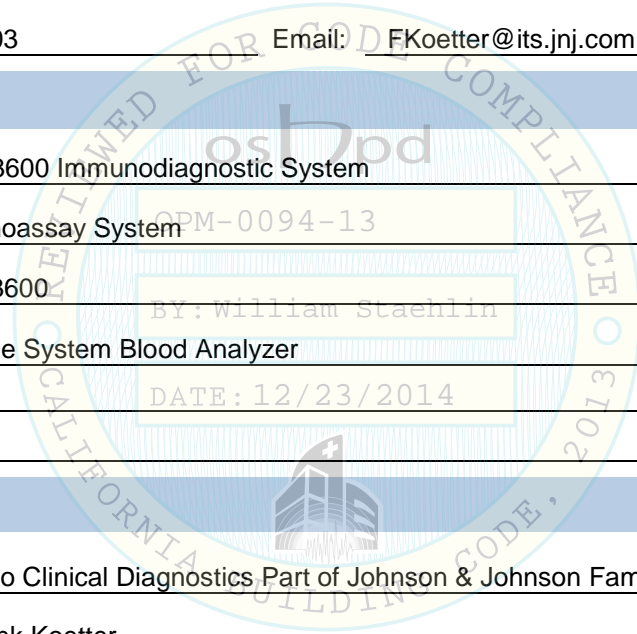


Applicant Information

Applicant Company Name: Ortho Clinical Diagnostics Part of Johnson & Johnson Family of Companies
Contact Person: Frank Koetter
Mailing Address: 100 Indigo Creek Drive, MC00891, Rochester, NY 14626-5101
Telephone: 1-585-453-4003 Email: FKoetter@its.jnj.com

I hereby agree to reimburse the Office of Statewide Health Planning and Development review fees in accordance with the California Administrative Code, 2013.

Signature of Applicant: [Signature] Date: 4/22/14
Title: Group Director, Systems Development & LCM Company Name: Ortho Clinical Diagnostics





**OFFICE OF STATEWIDE HEALTH PLANNING AND DEVELOPMENT  
FACILITIES DEVELOPMENT DIVISION**

**Registered Design Professional Preparing Engineering Recommendations**

Company Name: CYS Structural Engineers, Inc.

Name: Dieter T. Siebald California License Number: S.E. #4346

Mailing Address: 2495 Natomas Park Drive, Suite 650, Sacramento, CA 95833

Telephone: 916-920-2020 Email: dieters@cyseng.com

**OSHPD Special Seismic Certification Preapproval (OSP)**

- Special Seismic Certification is preapproved under OSP- (Separate application for OSP is required)
- Special Seismic Certification is not preapproved

**Certification Method(s)**

- Testing in accordance with:  ICC-ES AC156  FM 1950-10
- Other\* (Please Specify): \_\_\_\_\_

\*Use of criteria other than those adopted by the California Building Standards Code, 2013 (CBSC 2013) for component supports and attachments are not permitted. For distribution system, interior partition wall, and suspended ceiling seismic bracings, test criteria other than those adopted in the CBSC 2013 may be used when approved by OSHPD prior to testing.

- Analysis
- Experience Data
- Combination of Testing, Analysis, and/or Experience Data (Please Specify): \_\_\_\_\_

**List of Attachments Supporting the Manufacturer's Certification**

- Test Report  Drawings  Calculations  Manufacturer's Catalog
- Other(s) (Please Specify): \_\_\_\_\_

**OFFICE USE ONLY – OSHPD APPROVAL VALID FOR CBC 2013 ONLY**


Signature: *William Staehlin* Date: 12/23/2014

Print Name: William Staehlin

Title: SSE

Condition of Approval (if applicable): \_\_\_\_\_


"Access to Safe, Quality Healthcare Environments that Meet California's Diverse and Dynamic Needs"



OPM-0094-13  
TABLE OF CONTENTS

	PAGE
GENERAL NOTES .....	2
ABBREVIATIONS & DESIGN CRITERIA .....	5
VITROS 3600	
PLAN & ELEVATION .....	6
FRONT BRACKET ASSEMBLY DETAIL .....	7
FRONT FRAME BRACKET DETAIL .....	8
FRONT FLOOR BRACKET DETAIL .....	9
REAR BRACKET ASSEMBLY DETAIL .....	10
REAR FRAME BRACKET DETAIL .....	11
REAR FLOOR BRACKET DETAIL .....	12
ATTACHMENT DETAIL TO CONCRETE FILL OVER METAL DECK .....	13
ATTACHMENT DETAIL TO CONCRETE SLAB .....	17

- NOTES:**
1. THESE DRAWINGS ARE PREPARED FOR ORTHO CLINICAL DIAGNOSTICS, ROCHESTER, NEW YORK.
  2. THE CONTRACTOR AND INSPECTOR OF RECORD SHALL OBTAIN A COPY OF THIS PRE-APPROVAL FROM THE OSHPD PRE-APPROVAL PROGRAMS WEBSITE.
  3. THIS PRE-APPROVAL COVERS THE SUPPORTS AND ATTACHMENTS OF THE COMPONENT (EQUIPMENT) TO THE SUPPORTING STRUCTURE. THE UNIT AND ATTACHMENT HARDWARE ARE SUPPLIED BY ORTHO CLINICAL DIAGNOSTICS. THROUGH BOLTS, UNDER FLOOR HARDWARE AND ATTACHMENTS AT SOFFIT UNDER METAL DECK AND EXPANSION BOLTS SHOWN ON PAGES 13 THRU 18 SHALL BE SUPPLIED AND INSTALLED BY THE CONTRACTOR.

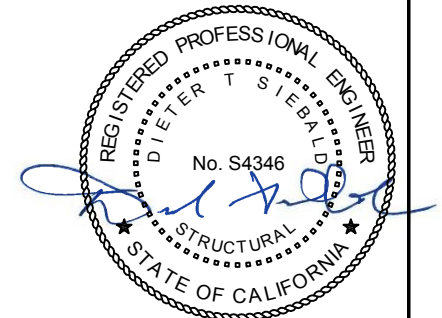


SHEET TITLE: TABLE OF CONTENTS

 <p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 1 of 18
--	--------------------------------------	---

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:30pm Login:cmachom DimScale:1 L1Scale:6

**GENERAL NOTES:**

1. THIS OSHPD PRE-APPROVAL OF MANUFACTURER'S CERTIFICATION (OPM) IS BASED ON THE CBC 2013. THE DEMAND (DESIGN FORCES) FOR USE WITH THIS OPM SHALL BE BASED ON THE CBC 2013.
2. IT IS THE RESPONSIBILITY OF THE STRUCTURAL ENGINEER OF RECORD FOR A SITE SPECIFIC PROJECT TO VERIFY:
  - A. THE ADEQUACY OF THE NEW OR EXISTING STRUCTURE TO RESIST THE FORCES AND WEIGHT SPECIFIED FOR EACH EQUIPMENT IN ADDITION TO ALL OTHER LOADS. PROVIDE AND DESIGN SUPPLEMENTARY MEMBERS AS REQUIRED.
  - B. THAT THE FLOOR ANCHORS ARE LOCATED AT AN ADEQUATE DISTANCE FROM ANY SLAB EDGES OR OPENINGS.
  - C. THAT THE FLOOR ANCHORS ARE LOCATED AT AN ADEQUATE DISTANCE FROM ANY NEW OR EXISTING ANCHORS. THE SPACING SHOWN IN THE TEST LOADS TABLE ON PAGE 3 IS THE REQUIRED MINIMUM SPACING OF THE 1/2" DIAMETER ANCHOR BOLTS. THE REQUIRED SPACING FROM ANCHORS OF OTHER DIAMETERS AND EMBEDMENTS MAY VARY AND SHALL BE EVALUATED BY THE SEOR.
  - D. THAT THE INSTALLATION IS IN CONFORMANCE WITH THE CBC 2013 AND WITH THE DETAILS SHOWN IN THIS PRE-APPROVAL.
  - E. THAT THE ACTUAL EQUIPMENT'S WEIGHT, CENTER OF GRAVITY (CG) LOCATION, ANCHOR LOCATIONS, ANCHOR DETAILS, AND THE MATERIAL AND GAGE OF THE EQUIPMENT WHERE ATTACHMENTS ARE MADE, AGREE WITH THE INFORMATION SHOWN ON THE PRE-APPROVAL DOCUMENTS.
  - F. THAT THE PROJECT SPECIFIC VALUES OF  $S_{DS}$  &  $z/h$  RESULT IN SEISMIC FORCES ( $E_h$ ,  $E_v$ ) THAT DO NOT EXCEED THE VALUES IN THE DETAILS.
- 3A. EXPANSION ANCHORS INSTALLED IN NORMAL WEIGHT OR SAND-LIGHTWEIGHT CONCRETE SHALL BE CARBON STEEL HILTI KB-TZ EXPANSION ANCHORS COMPLYING WITH ESR-1917 REISSUED MAY 1, 2013.
- B. INSTALLATION: INSTALL THE EXPANSION ANCHORS IN ACCORDANCE WITH THE REQUIREMENTS GIVEN IN THE ICC EVALUATION REPORT FOR THE SPECIFIC ANCHOR AND THE PARAMETERS GIVEN IN THE TABLE ON PAGE 3.
- C. JOB TESTING: FOR VERIFYING SATISFACTORY INSTALLATION WORKMANSHIP, PERFORM JOB SITE TESTING IN ACCORDANCE WITH THE TEST LOAD VALUES GIVEN IN THE TABLE ON PAGE 3. TEST 50% OF THE INSTALLED ANCHORS. THE TEST LOAD MAY BE APPLIED BY ANY METHOD THAT WILL EFFECTIVELY MEASURE THE TENSION IN THE ANCHOR SUCH AS DIRECT PULL WITH A HYDRAULIC JACK OR CALIBRATED SPRING LOADING DEVICES OR CALIBRATED TORQUE WRENCH METHOD. ALL TESTS SHALL BE CONDUCTED IN THE PRESENCE OF THE INSPECTOR OF RECORD. REPORT OF TEST RESULTS TO BE SUBMITTED TO OSHPD. IF ANY ANCHOR FAILS THE TEST, TEST ALL ANCHORS. THE TEST SHALL BE PERFORMED 24 HOURS OR MORE AFTER INSTALLATION. TESTING MAY BE DONE PRIOR TO EQUIPMENT INSTALLATION. ALSO REFER TO CBC 1913A.7 "FIELD TESTS FOR POST-INSTALLED ANCHORS IN CONCRETE".
- D. FAILURE/ACCEPTANCE CRITERIA: THE FOLLOWING CRITERIA APPLY FOR THE ACCEPTANCE OF INSTALLED ANCHORS:
  - HYDRAULIC RAM METHOD: APPLY AND HOLD TEST LOAD FOR A MINIMUM OF 15 SECONDS. THE ANCHOR SHOULD HAVE NO OBSERVABLE MOVEMENT AT THE APPLICABLE TEST LOAD WHERE WASHERS ARE USED. FOR WEDGE TYPE ANCHORS, SUCH AS HILTI KB-TZ, A PRACTICAL WAY TO DETERMINE OBSERVABLE MOVEMENT IS THAT THE WASHER UNDER THE NUT BECOMES LOOSE.
  - TORQUE WRENCH METHOD: THE APPLICABLE TEST TORQUE MUST BE REACHED WITHIN THE FOLLOWING LIMITS: WEDGE TYPE: ONE-HALF (1/2) TURN OF THE NUT.

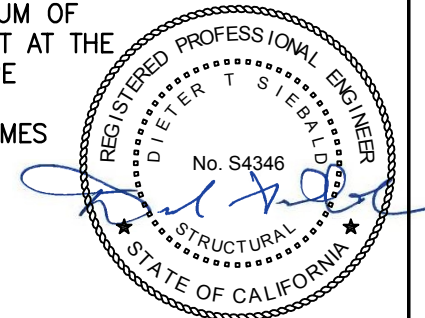

SHEET TITLE: GENERAL NOTES



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833


TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	2 of 18

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:31pm Login:camachom Dimscaler:1 L1Scale:6

**GENERAL NOTES CONTINUED:**

3E. TEST VALUES: APPLY TEST LOADS TO ANCHORS WITHOUT REMOVING THE NUT IF POSSIBLE, SEE TABLE BELOW.

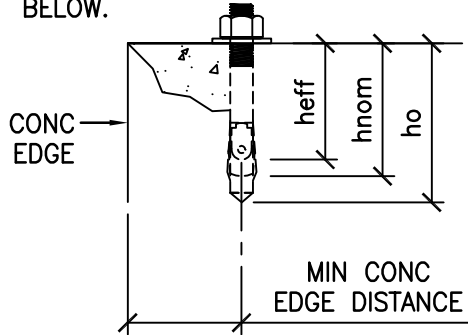

ANCHOR DIA (INCH) da	INSTALLATION EMBED (INCH) hnom	EFFECTIVE EMBED (INCH) hef	HOLE DEPTH (INCH) ho	MIN CONC THICKNESS (INCH) h <sub>min</sub>	MIN CONC EDGE DISTANCE (INCH)	MIN AB SPACING (INCH)	TEST LOAD		CONDITION OF ANCHORAGE
							TENSION LOAD (LBS)	TORQUE (FT-LBS)	
1/2	2 3/8	2	2 5/8	4	12	4	1866	40	CASE 3
1/2	3 5/8	3 1/4	4	6	12	4	3407	40	CASE 2

4. BOLTS THROUGH CONCRETE ON METAL DECK:

- A. BOLTS SHALL BE TORQUED BY 3/4 TURN OF THE NUTS AFTER SNUG TIGHT (THE SNUG TIGHT CONDITION IS DEFINED AS THE TIGHTNESS REQUIRED TO BRING THE CONNECTED PLIES INTO FIRM CONTACT) CONDITION IS ACHIEVED, UNLESS NOTED OTHERWISE.
- B. THROUGH BOLT HOLES SHALL BE 1/16" LARGER THAN BOLT SIZE (HOLE SIZE = BOLT SIZE + 1/16")
- C. THROUGH BOLTS IN CONCRETE SHALL RECEIVE SPECIAL INSPECTION & TESTING (THROUGH BOLTS WITH STEEL TO STEEL CONNECTION IN TENSION DO NOT REQUIRE TESTING) IN ACCORDANCE WITH REQUIREMENTS FOR POST-INSTALLED ANCHORS.

5. SCREW ANCHORS TO BOTTOM OF CONCRETE FILL OVER METAL DECK:

- A. HILTI KH-EZ (ICC ESR-3027) TENSION TEST LOAD FOR CASE 1.

ANCHOR DIA (INCH) da	INSTALLATION EMBED (INCH) hnom	EFFECTIVE EMBED (INCH) hef	HOLE DEPTH (INCH) ho	MIN CONC THICKNESS (INCH) h <sub>min</sub>	MIN CONC EDGE DISTANCE (INCH)	MIN AB SPACING (INCH)	TENSION TEST LOAD (LBS)
1/4	1 5/8	1.18	2	3/4	1 1/4*	10*	400

\* SEE PAGE 14 OF 18 IN THIS OPM.



SHEET TITLE: GENERAL NOTES (CONTINUED)



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833


TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	3 of 18



**GENERAL NOTES CONTINUED:**

6. THREE (3) CASES OF ANCHORAGE ARE SPECIFIED AND PRESENTED IN THIS PRE-APPROVAL:


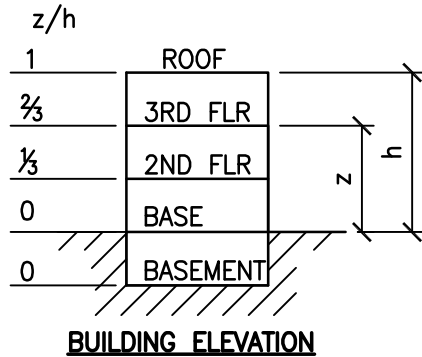


**CASE 1:** ANCHORAGE DETAILS LOCATED AT UPPER FLOORS ABOVE THE BASE OF A BUILDING ( $z/h \leq 1.0$ ), IT IS ASSUMED THAT THE FLOORS ARE BUILT OF A MINIMUM 3/4" SAND-LIGHTWEIGHT CONCRETE TOPPING OVER METAL DECK ( $f'c = 3000$  PSI, MINIMUM).

**CASE 2:** ANCHORAGE DETAILS LOCATED AT OR BELOW THE BASE OF A BUILDING ( $z/h = 0$ ). THE FLOORS ARE ASSUMED TO BE BUILT OF A MINIMUM 6" NORMAL-WEIGHT CONCRETE SLAB ( $f'c = 3000$  PSI, MINIMUM).

**CASE 3:** ANCHORAGE DETAILS LOCATED AT OR BELOW THE BASE OF THE BUILDING ( $z/h = 0$ ). THE FLOORS ARE ASSUMED TO BE BUILT OF A MINIMUM 4" NORMAL-WEIGHT CONCRETE SLAB ( $f'c = 3000$  PSI, MINIMUM). **FOR THIS CASE THE MAXIMUM  $S_{DS}$  IS LIMITED TO 2.30.**

7. THIS PRE-APPROVAL MAY BE USED AT ANY GEOGRAPHICAL LOCATION IN THE STATE OF CALIFORNIA. WHERE  $S_{DS}$  IS LESS THAN OR EQUAL TO 2.50, **EXCEPT FOR CASE 3 ANCHORAGE WHERE  $S_{DS}$  MUST BE LESS THAN OR EQUAL TO 2.30.**

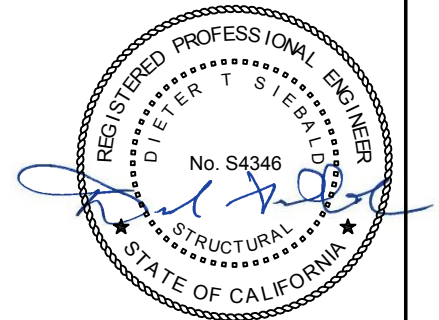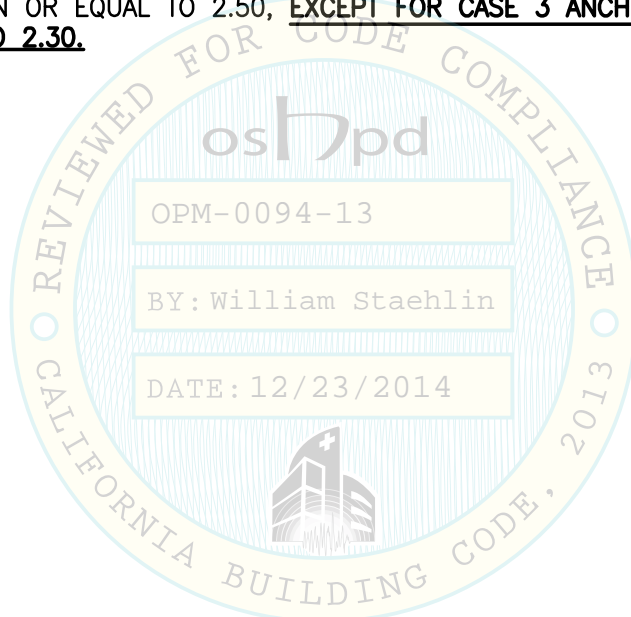

SHEET TITLE: GENERAL NOTES (CONTINUED)



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833


TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	4 of 18

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:31pm Login:cmachom Dimscaler:1 LTScale:6

**ABBREVIATIONS:**

AB	ANCHOR BOLTS	IN (")	INCH
ABV	ABOVE	KSI	KIPS PER SQUARE INCH
ADJ	ADJACENT	LRFD	LOAD AND RESISTANCE FACTOR DESIGN
ASTM	AMERICAN SOCIETY FOR TESTING & MATERIALS	LWC	LIGHT WEIGHT CONCRETE
BLW	BELOW	MAX	MAXIMUM
BOTT	BOTTOM	MFR	MANUFACTURER
CBC	CALIFORNIA BUILDING CODE	MIN	MINIMUM
CG	CENTER OF GRAVITY	MTL	METAL
☐	CENTERLINE	NO. (#)	NUMBER OR POUNDS
COORD	COORDINATE	NWC	NORMAL WEIGHT CONCRETE
CONC	CONCRETE	OSHPD	OFFICE OF STATEWIDE HEALTH PLANNING & DEVELOPMENT
DBL	DOUBLE	PG(S)	PAGE(S)
DIA (φ)	DIAMETER	☐	PLATE
(E)	EXISTING CONDITION	PSI	POUNDS PER SQUARE INCH
EA	EACH	SEOR	STRUCTURAL ENGINEER OF RECORD
ELEV	ELEVATION	STL	STEEL
EMBED	EMBEDMENT	T&B	TOP & BOTTOM
EQUIP	EQUIPMENT	Tu	ANCHORAGE TENSION REACTION DUE TO SEISMIC FORCE AT LRFD
f'c	MINIMUM ULTIMATE COMPRESSIVE STRENGTH OF CONCRETE	THRD	THREAD OR THREADED
FLR	FLOOR	TYP	TYPICAL
Fp	HORIZONTAL SEISMIC FORCE PER ASCE 7-10 SEISMIC FORCE REQUIREMENTS	VERT	VERTICAL
Fv	VERTICAL SEISMIC FORCE PER ASCE 7-10 SEISMIC FORCE REQUIREMENTS	Vu	ANCHORAGE SHEAR REACTION DUE TO SEISMIC FORCE AT LRFD
Fy	SPECIFIED YIELD STRENGTH OF STEEL, KSI	W/	WITH
GA	GAUGE	W/O	WITHOUT
		Wp	OPERATING WEIGHT

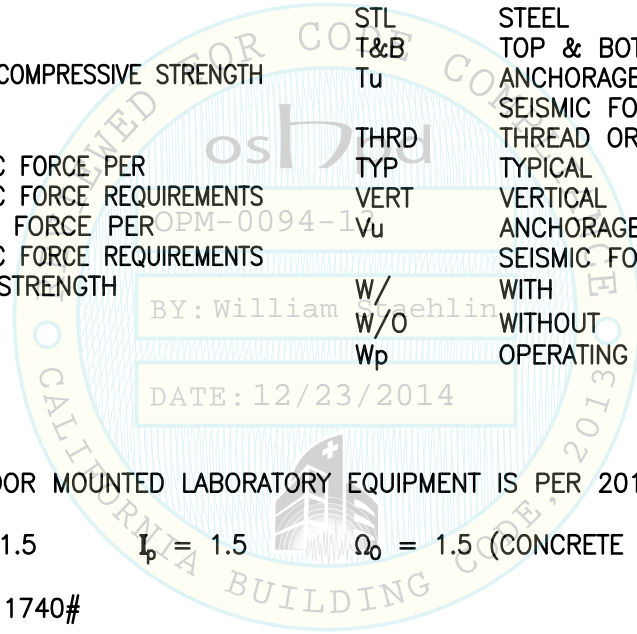

BY: William Staehlin  
DATE: 12/23/2014

**DESIGN CRITERIA**

ANCHORAGE DESIGN FOR FLOOR MOUNTED LABORATORY EQUIPMENT IS PER 2013 CBC AT LRFD LEVEL FORCES

$\alpha_p = 1.0$        $R_p = 1.5$        $I_p = 1.5$        $\Omega_0 = 1.5$  (CONCRETE ANCHORS)

VITROS 3600:       $W_p = 1740\#$

FOR CASE 1 – UPPER FLOORS ABOVE THE BASE,  $z/h \leq 1.0$


$S_{Ds} = 2.50$        $F_p = 3.0 W_p$        $F_v = 0.50 W_p$

FOR CASE 2 – SLAB AT OR BELOW BASE,  $z/h = 0$

$S_{Ds} = 2.50$        $F_p = 1.125 W_p$        $F_v = 0.50 W_p$

FOR CASE 3 – SLAB AT OR BELOW BASE,  $z/h = 0$

$S_{Ds} = 2.30$        $F_p = 1.035 W_p$        $F_v = 0.46 W_p$

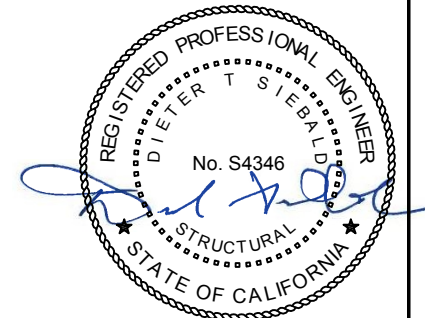

SHEET TITLE: ABBREVIATIONS  
DESIGN CRITERIA



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com



Job No: 13072.02  
Date: 12/19/2014  
Page: 5 of 18

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:31pm Login:cmachom Dimscaler:1 LTScale:6


VITROS 3600 IMMUNODIAGNOSTICS SYSTEM  
EQUIPMENT ATTACHMENT

Ortho Clinical Diagnostics

PART OF THE *Johnson & Johnson* FAMILY OF COMPANIES

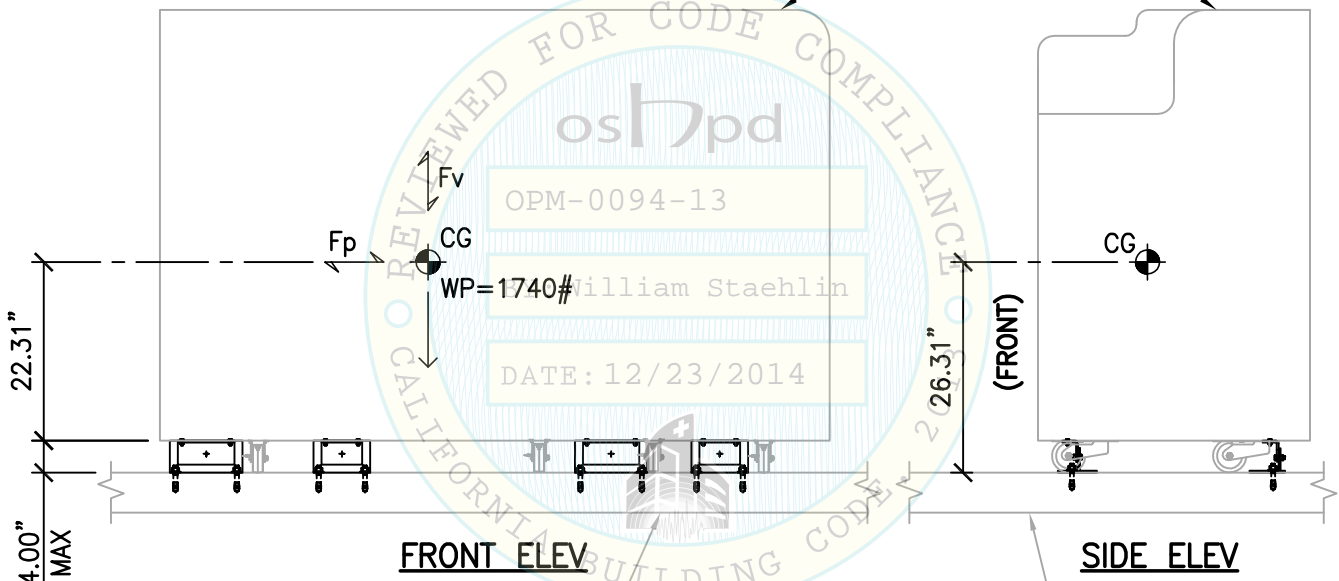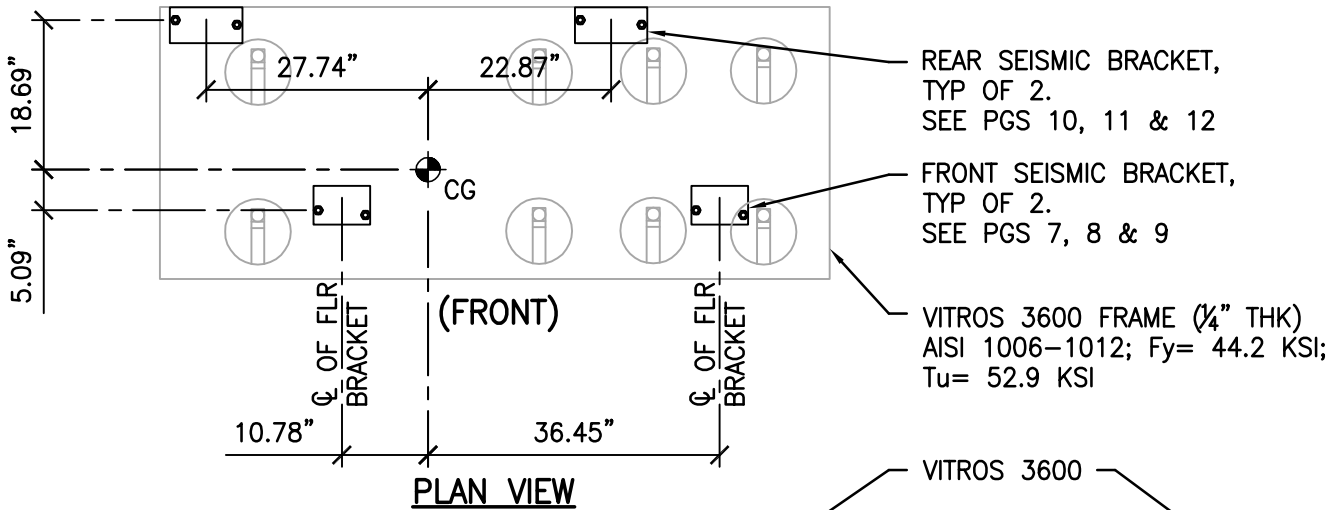

(E) SUPPORTING STRUCTURE.  
SEE PGS 13, 14, 17 OR 18  
AS APPLICABLE

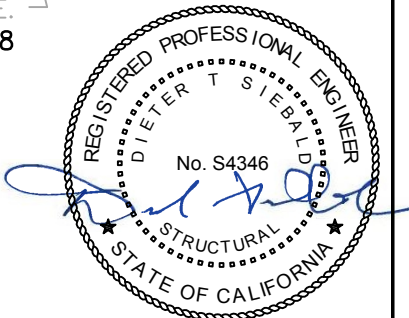


SHEET TITLE: PLAN & ELEVATION



<p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 6 of 18
--	--------------------------------------	---

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:31pm Login:cammachom Dimstyle:1 LTScale:6



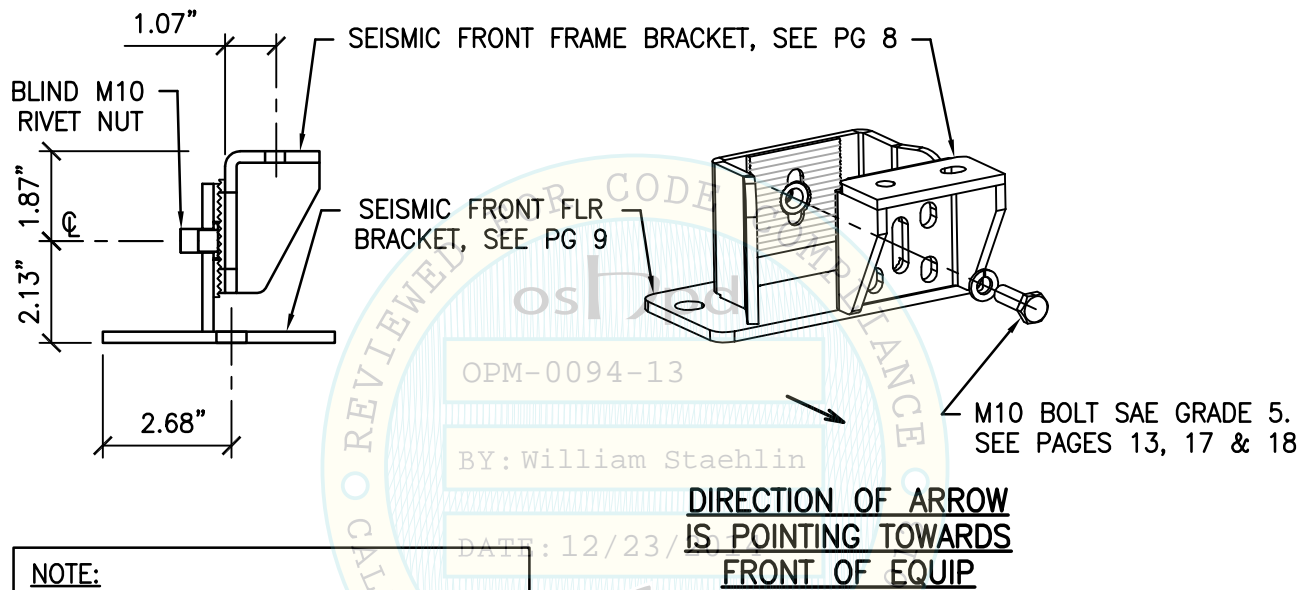

**NOTE:**  
BRACKET MATERIAL IS AISI 1006/1012  
LOW CARBON STEEL ( $F_y = 44$  KSI).  
SERRATED PLATE MATERIAL IS ASTM  
A516 GRADE 60.

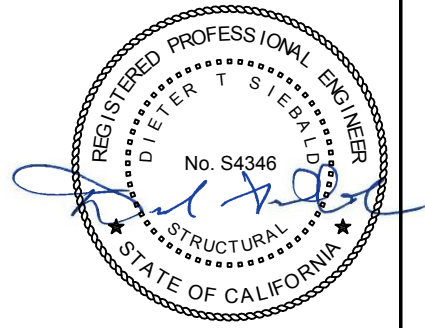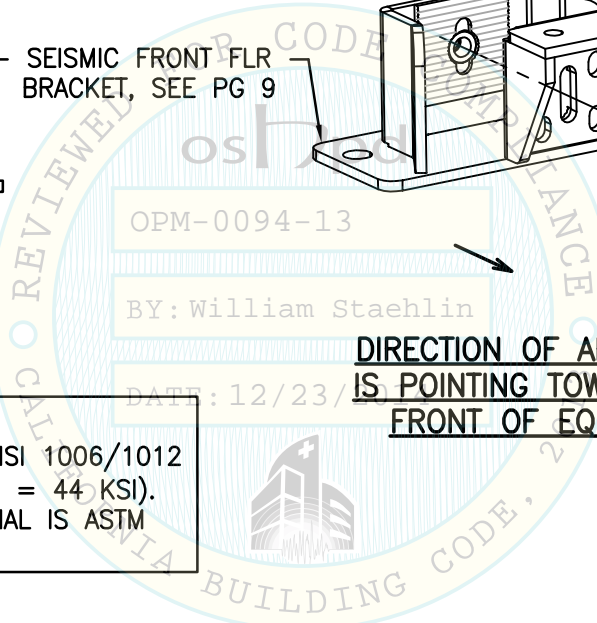

SHEET TITLE: FRONT BRACKET ASSEMBLY DETAIL



**CYS STRUCTURAL ENGINEERS, INC.**




2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	7 of 18

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014-05:31pm Login:camachom Dimstyle:1 LTScale:6

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRUS1\_TASK 02.dwg Time:Dec19,2014-05:32pm Login:carmachom Dimstyle:1 LTScale:6

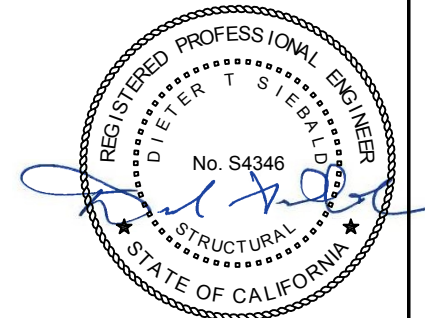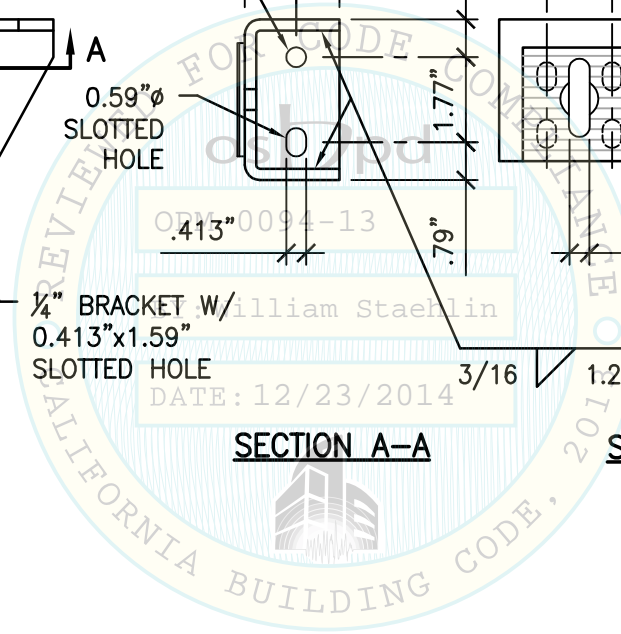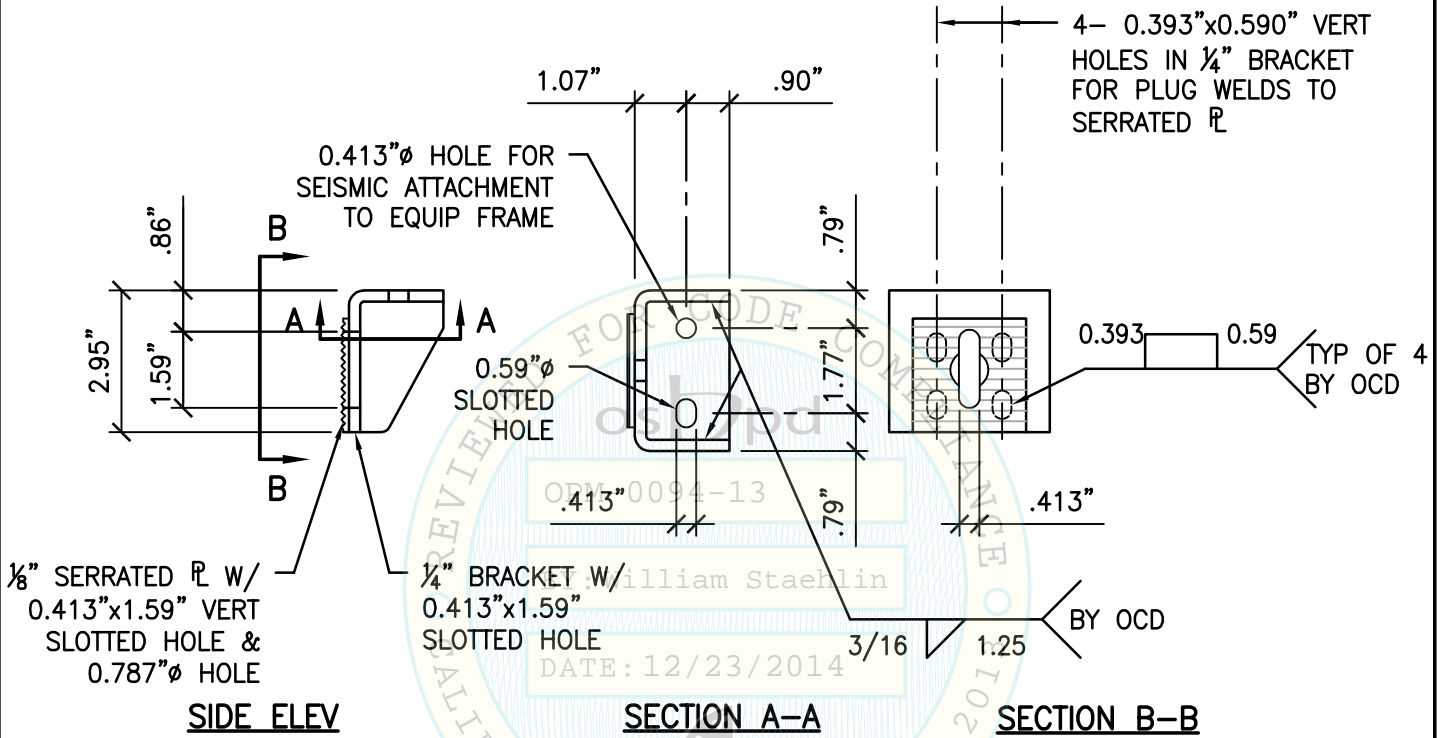


SHEET TITLE: FRONT FRAME BRACKET DETAIL

 <p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 8 of 18
--	--------------------------------------	---

VITROS 3600 IMMUNODIAGNOSTICS SYSTEM  
EQUIPMENT ATTACHMENT

Ortho Clinical Diagnostics

PART OF THE *Johnson & Johnson* FAMILY OF COMPANIES

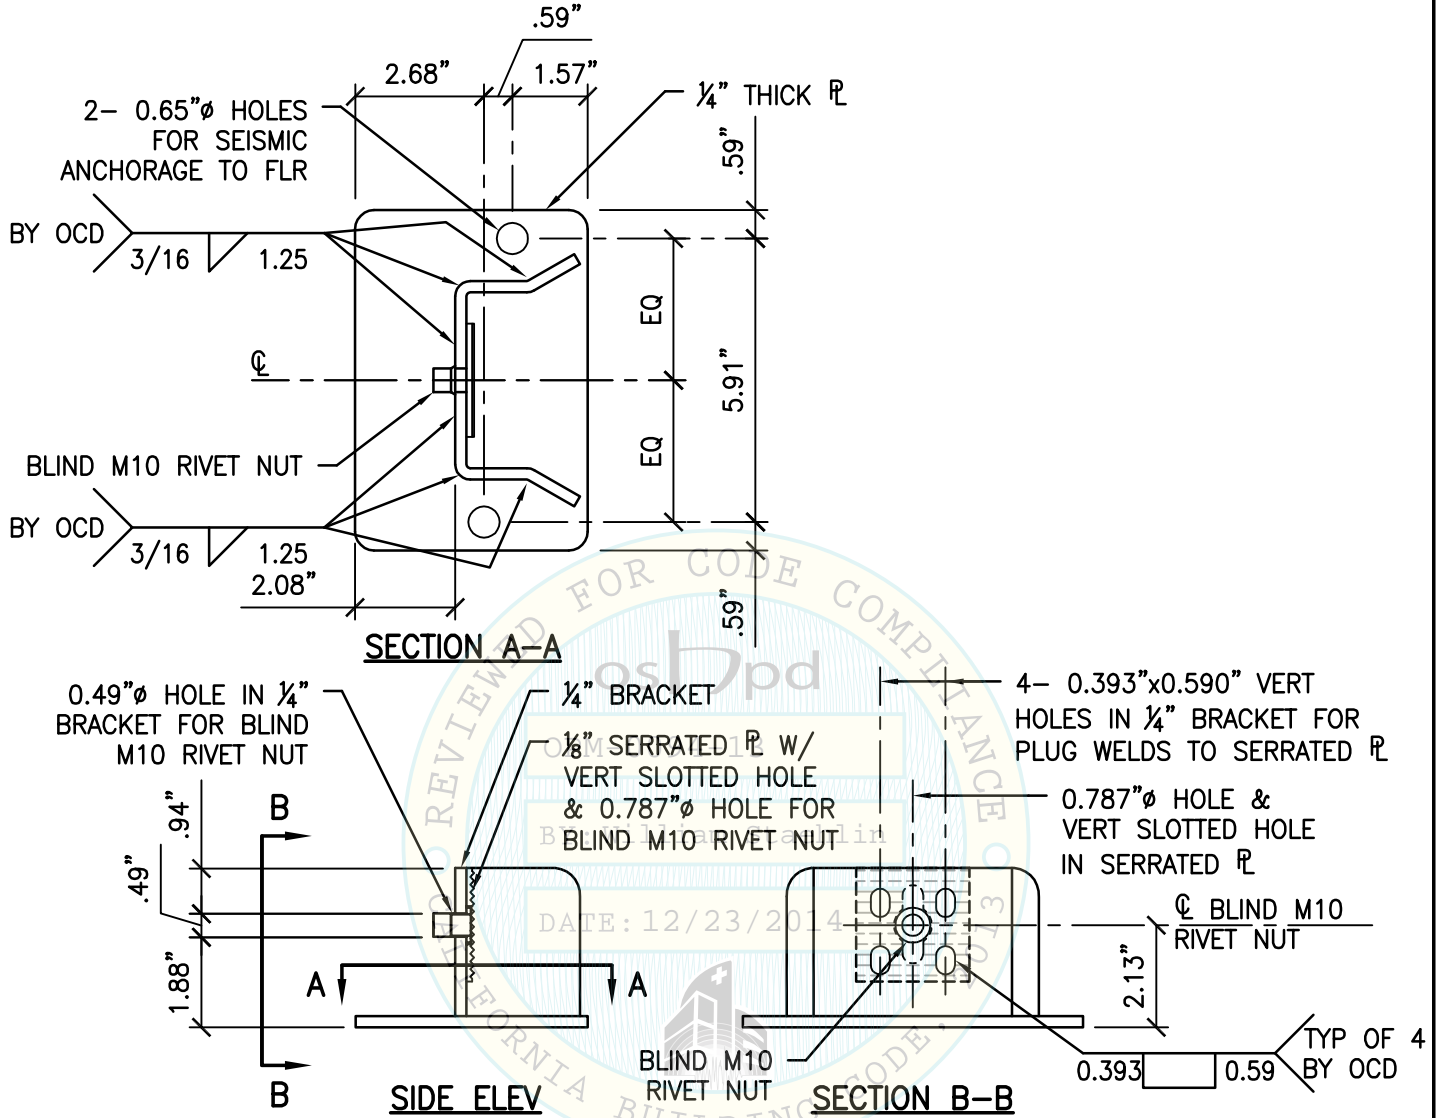


SHEET TITLE: FRONT FLOOR BRACKET DETAIL

<p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 9 of 18
--	--------------------------------------	---

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time: Dec 19, 2014 - 05:32pm Login: camachom Dimstyle: 1 LTScale: 6

**NOTE:**  
ONLY ONE REAR BRACKET  
ASSEMBLY HAS A LOCATOR PIN.

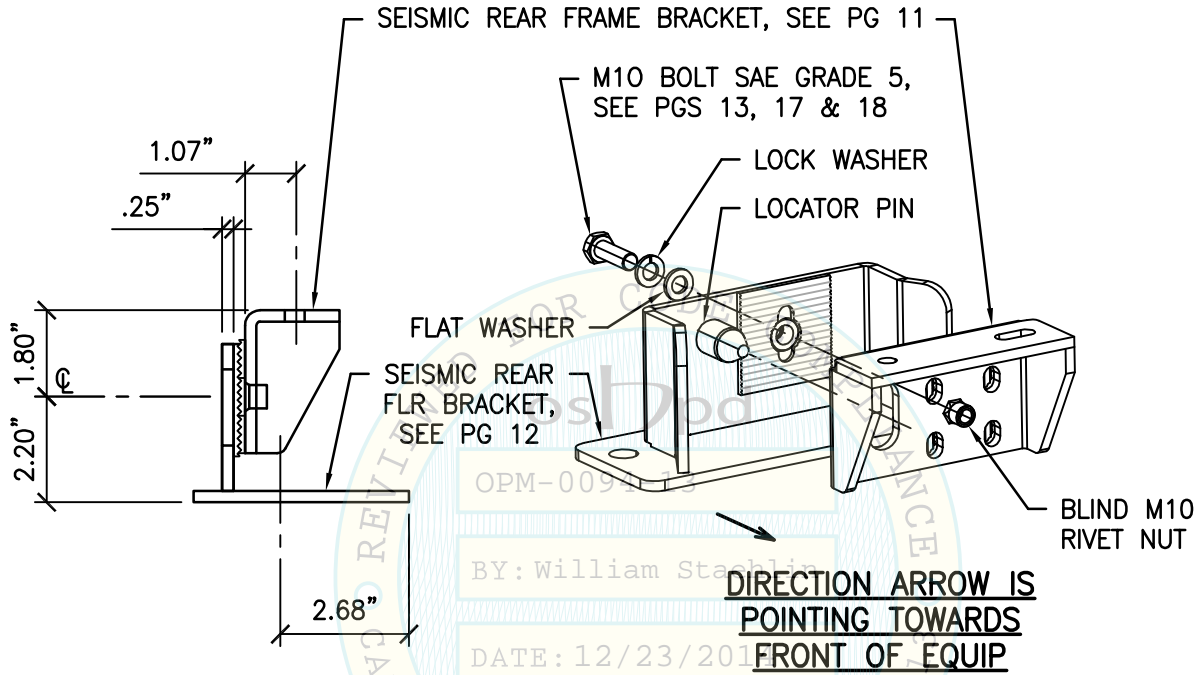

**NOTE:**  
BRACKET MATERIAL IS AISI 1006/1012  
LOW CARBON STEEL ( $F_y = 44$  KSI).  
SERRATED PLATE MATERIAL IS ASTM  
A516 GRADE 60.


OPM-0094-13

BY: William Staehlin

DATE: 12/23/2014

REVIEWED FOR CODE COMPLIANCE

BUILDING CODE, 2007

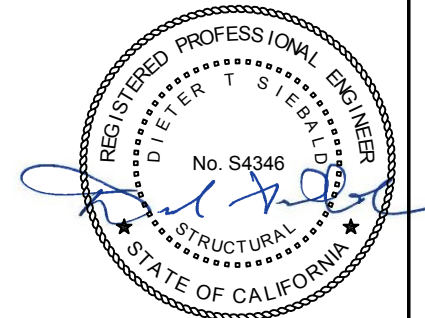

SHEET TITLE: REAR BRACKET ASSEMBLY DETAIL



**CYS STRUCTURAL ENGINEERS, INC.**




2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	10 of 18

L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:32pm Login:carmachom Dimstyle:1 LTScale:6



L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:32pm Logincamachom Dimscaler:1 LITScale:6

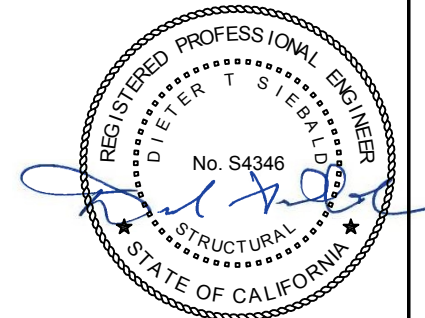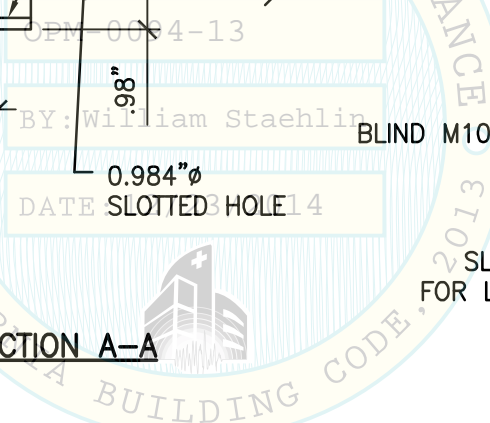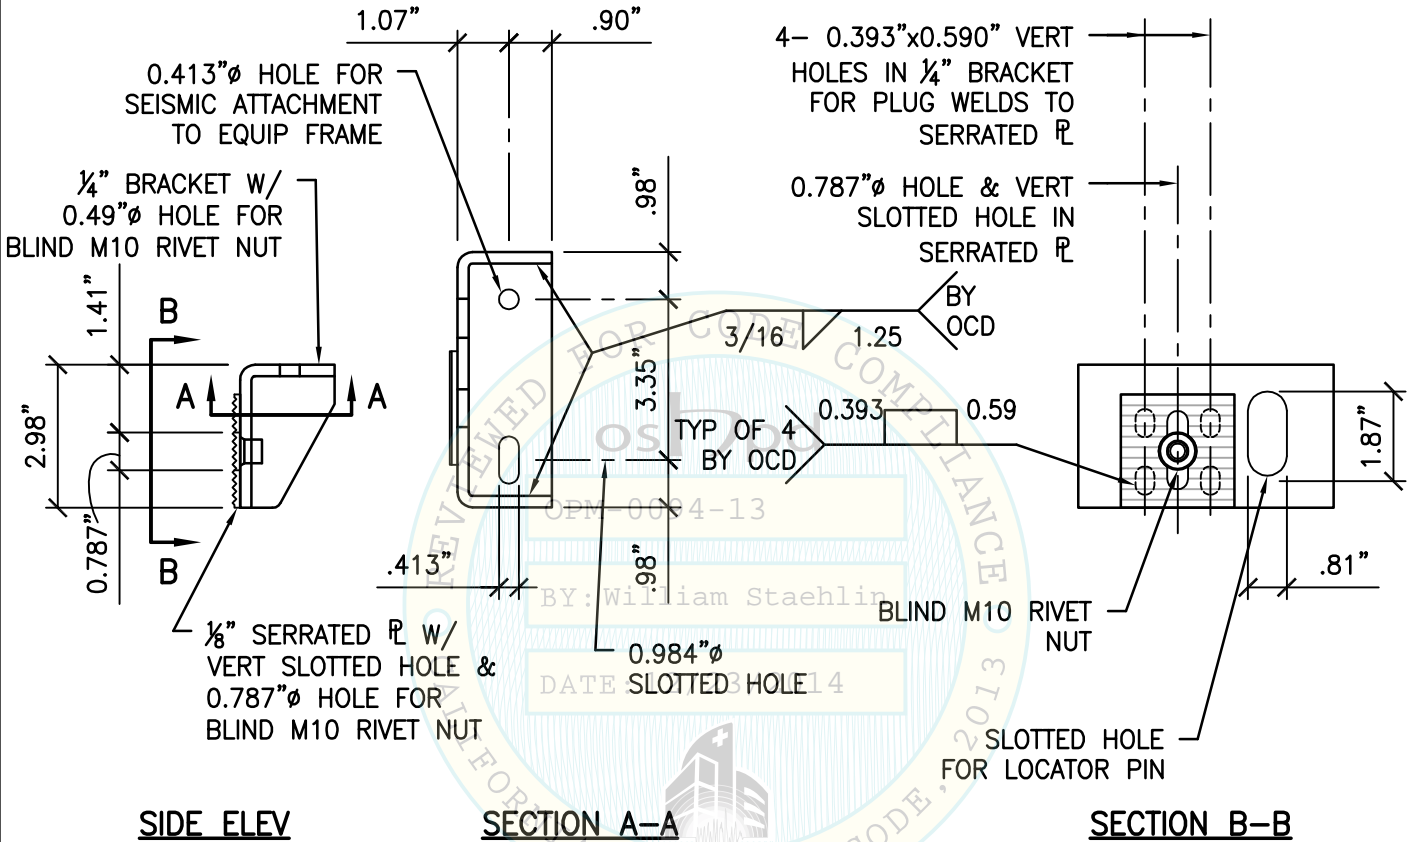


SHEET TITLE: REAR FRAME BRACKET DETAIL

 <b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 11 of 18
---	--------------------------------------	--



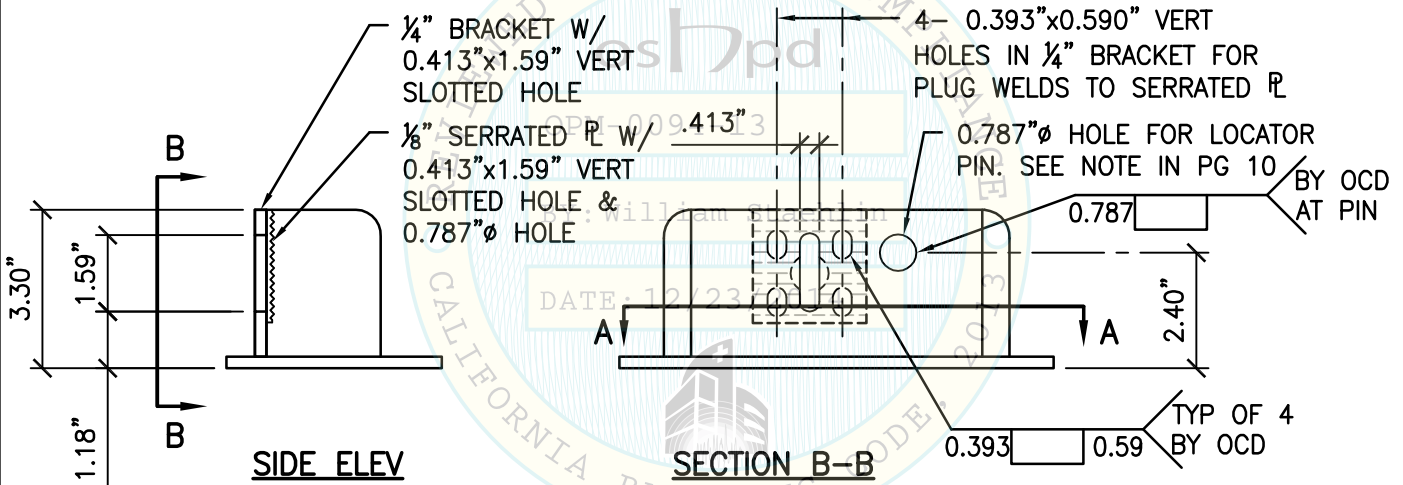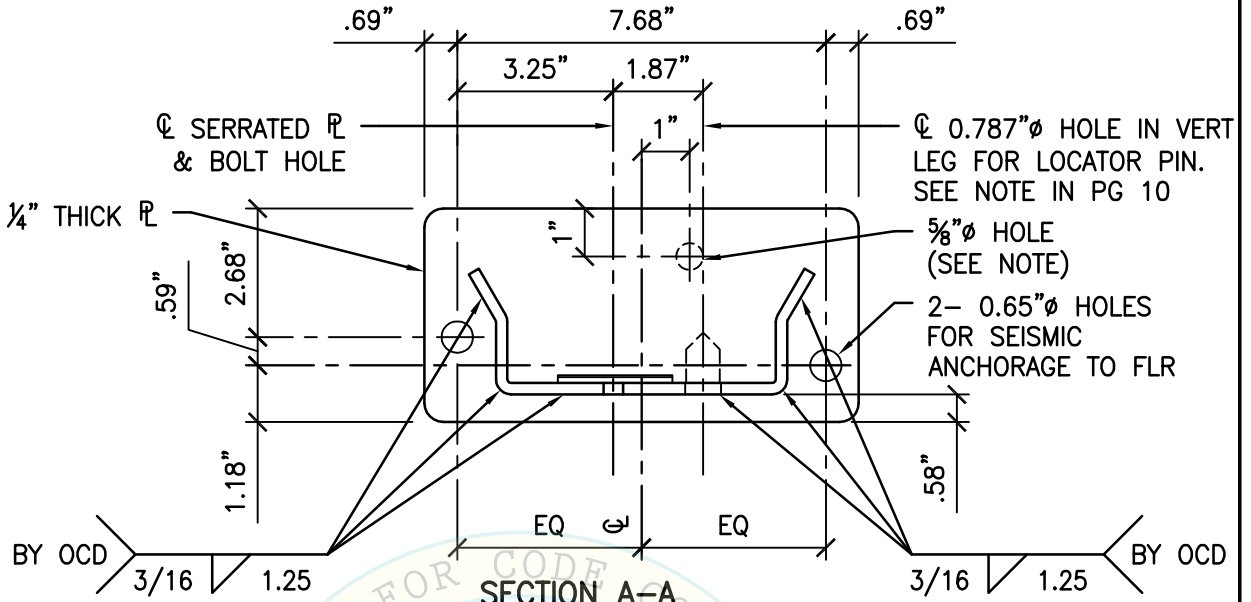

**NOTE:**  
FOR CASE 2 & CASE 3, ADDITIONAL ANCHORAGE HOLE MUST BE DRILLED THRU BRACKET BY THE CONTRACTOR TO ACCOMMODATE AN ADDITIONAL ANCHOR. CONTRACTOR IS RESPONSIBLE FOR REPLACING BRACKET IF IT IS DAMAGED DURING DRILLING.

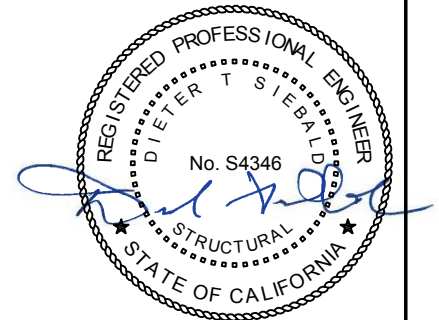

SHEET TITLE: REAR FLOOR BRACKET DETAIL

<p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 12 of 18
--	--------------------------------------	--



L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014-05:32pm Login:cmachom Dimstyle:1 LTScale:6

MAX ANCHOR FORCES AT LRFD AT EACH ANCHOR BOLT

FRONT BRACKET		REAR BRACKET	
Tu	Vu	Tu	Vu

CASE 1 z/h ≤ 1.0 W/O $\Omega_o$	2708#	813#	4644#	837#
CASE 1 z/h ≤ 1.0 W/ $\Omega_o$	2708#	1220#	4644#	1255#

( $\Omega_o = 1.5$ ) OVERSTRENGTH FACTOR  
MUST BE APPLIED TO SHEAR  
FORCE ONLY

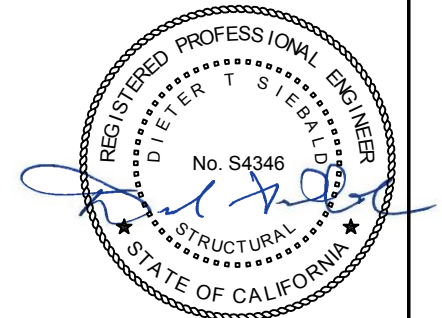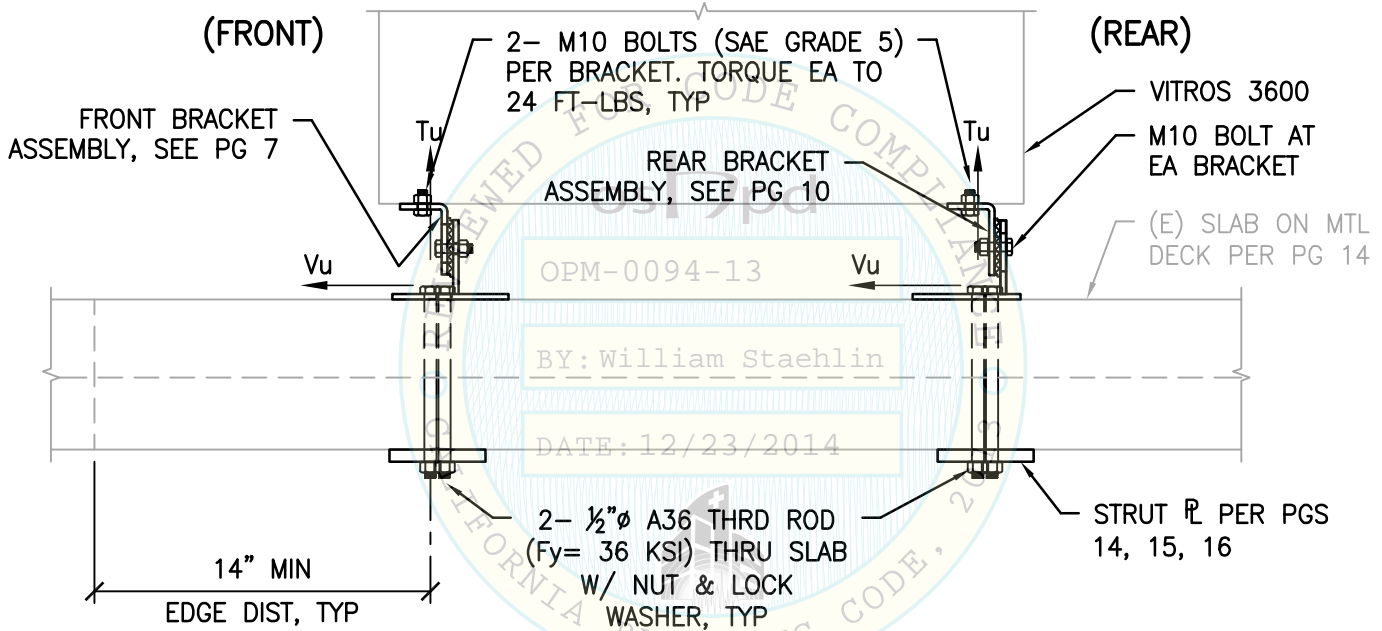

SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE FILL OVER METAL DECK





**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	13 of 18

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:32pm Login:camachom Dimstyle:1 LTScale:6

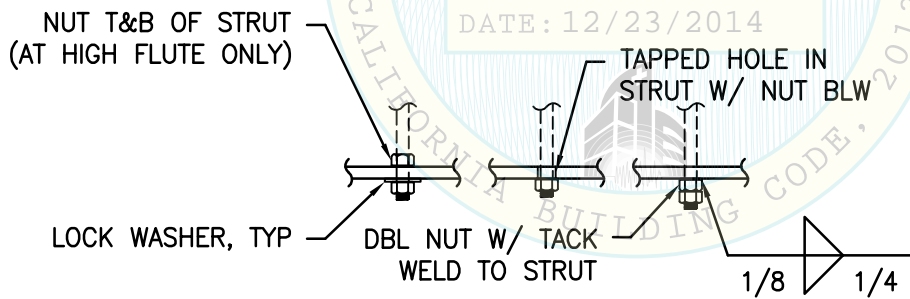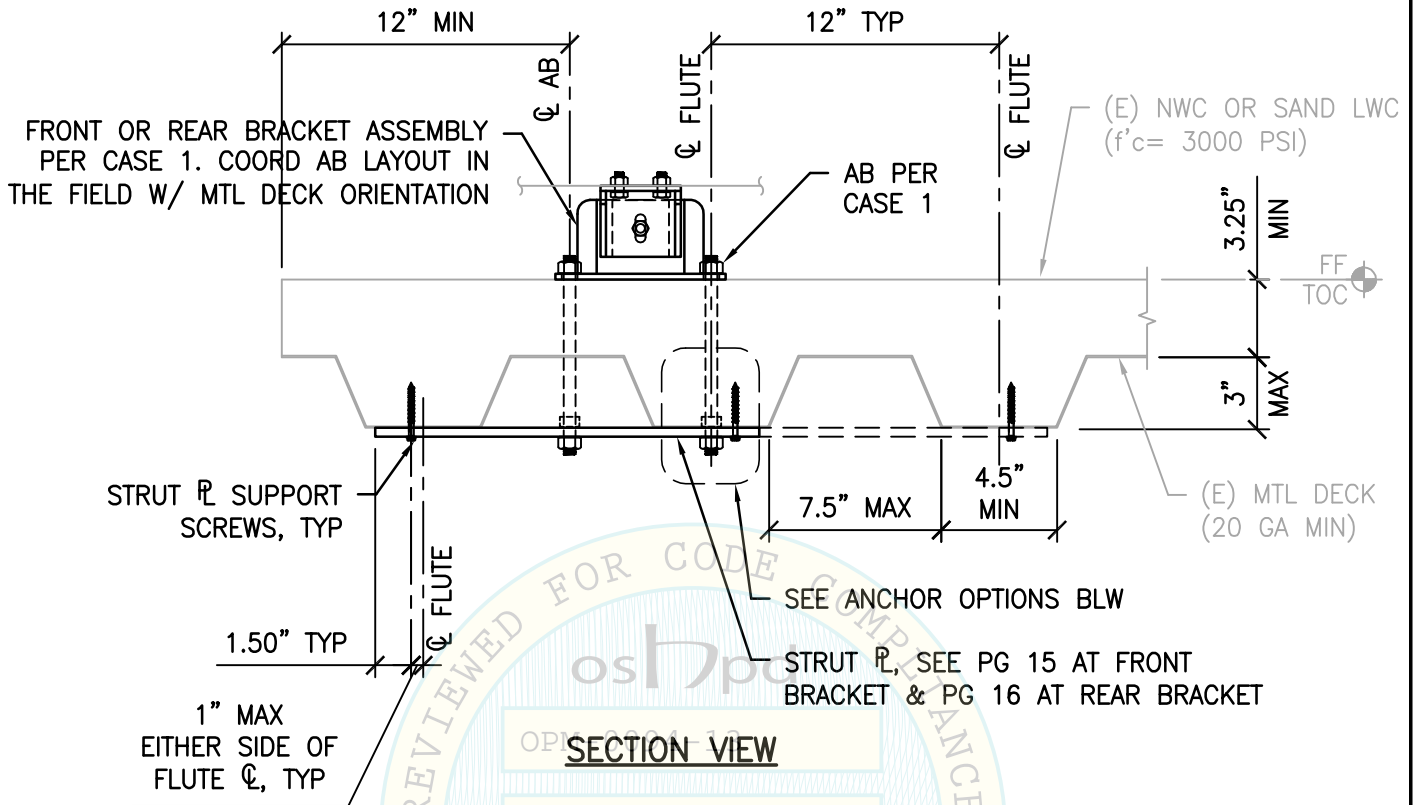

REVIEWED FOR CODE COMPLIANCE

BY: William Staehlin

DATE: 12/23/2014



SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE FILL OVER METAL DECK

<p><b>CYS STRUCTURAL ENGINEERS, INC.</b> 2495 NATOMAS PARK DRIVE, SUITE 650 SACRAMENTO, CA 95833</p>	TEL (916) 920-2020 www.cyseng.com	Job No: 13072.02 Date: 12/19/2014 Page: 14 of 18
--	--------------------------------------	--

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:53pm LogIn:camachom DimScale:1 L1Scale:6


VITROS 3600 IMMUNODIAGNOSTICS SYSTEM  
EQUIPMENT ATTACHMENT

Ortho Clinical Diagnostics

PART OF THE *Johnson & Johnson* FAMILY OF COMPANIES

EXTEND STRUT LENGTH TO  
NEXT ADJ LOW FLUTE IF AB'S  
ARE LESS THAN 2" FROM  
STRUT  $\bar{r}$  SUPPORT SCREWS

LENGTH SHALL  
ENGAGE  
2 LOW FLUTES MIN

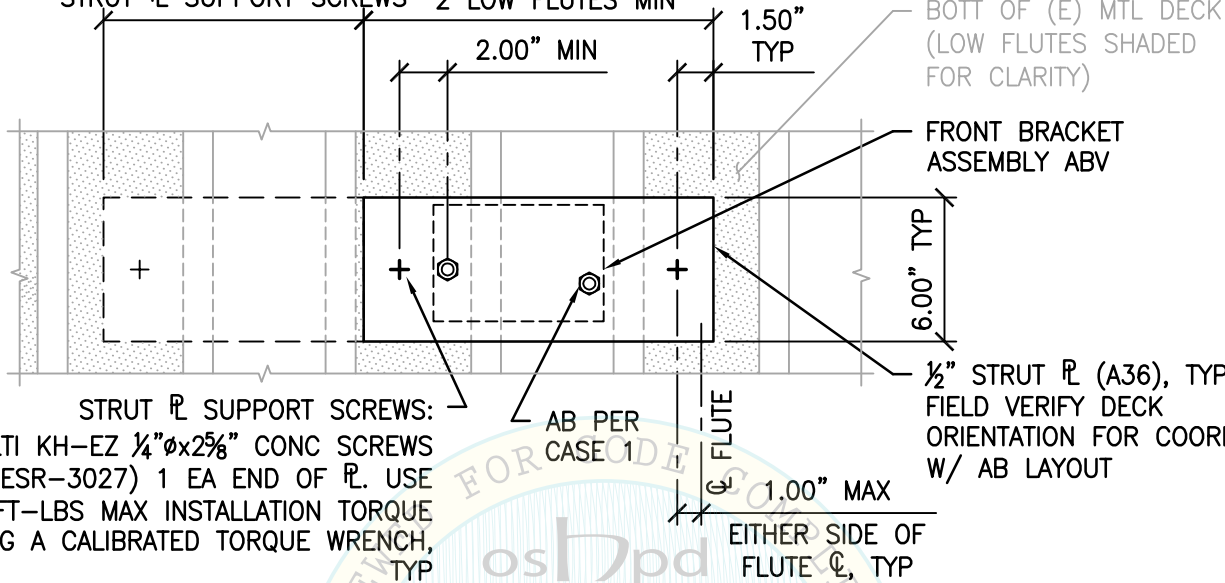

BOTT OF (E) MTL DECK  
(LOW FLUTES SHADED  
FOR CLARITY)

FRONT BRACKET  
ASSEMBLY ABV

$\frac{1}{2}$ " STRUT  $\bar{r}$  (A36), TYP.  
FIELD VERIFY DECK  
ORIENTATION FOR COORD  
W/ AB LAYOUT

STRUT  $\bar{r}$  SUPPORT SCREWS:  
HILTI KH-EZ  $\frac{1}{4}$ " $\phi$ x $2\frac{5}{8}$ " CONC SCREWS  
(ICC ESR-3027) 1 EA END OF  $\bar{r}$ . USE  
18 FT-LBS MAX INSTALLATION TORQUE  
USING A CALIBRATED TORQUE WRENCH,  
TYP

AB PER  
CASE 1


$\frac{1}{2}$ " FLUTE  
1.00" MAX  
EITHER SIDE OF  
FLUTE  $\bar{c}$ , TYP

**PLAN VIEW**

ANCHORS PERPENDICULAR TO FLUTES

EXTEND STRUT LENGTH TO  
NEXT ADJ LOW FLUTE IF AB'S  
ARE LESS THAN 2" FROM  
STRUT  $\bar{r}$  SUPPORT SCREWS

LENGTH SHALL ENGAGE  
2 LOW FLUTES MIN

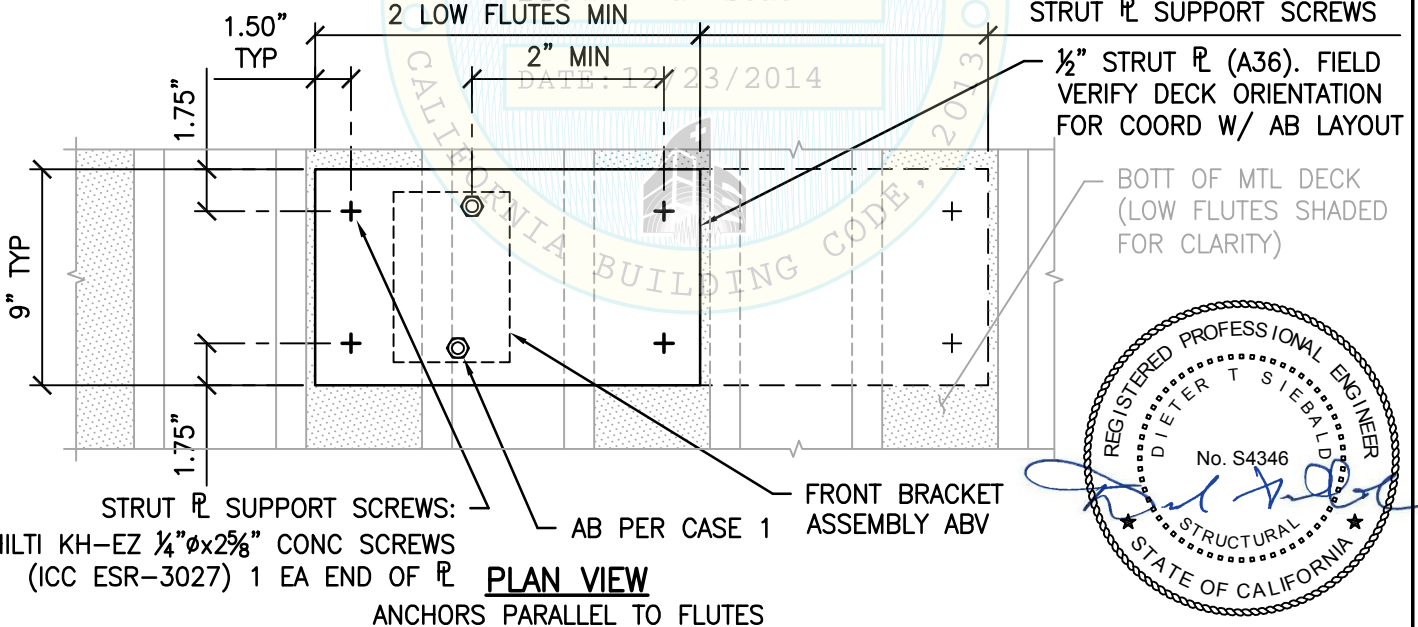

$\frac{1}{2}$ " STRUT  $\bar{r}$  (A36). FIELD  
VERIFY DECK ORIENTATION  
FOR COORD W/ AB LAYOUT

BOTT OF MTL DECK  
(LOW FLUTES SHADED  
FOR CLARITY)

STRUT  $\bar{r}$  SUPPORT SCREWS:  
HILTI KH-EZ  $\frac{1}{4}$ " $\phi$ x $2\frac{5}{8}$ " CONC SCREWS  
(ICC ESR-3027) 1 EA END OF  $\bar{r}$

AB PER CASE 1

FRONT BRACKET  
ASSEMBLY ABV

**PLAN VIEW**

ANCHORS PARALLEL TO FLUTES



SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE FILL OVER METAL DECK



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	15 of 18


L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRUS1\_TASK 02.dwg Time:Dec19,2014-05:33pm Login:camachom Dimscdle:1 L1Scale:6

VITROS 3600 IMMUNODIAGNOSTICS SYSTEM  
EQUIPMENT ATTACHMENT

Ortho Clinical Diagnostics

PART OF THE *Johnson & Johnson* FAMILY OF COMPANIES

EXTEND STRUT LENGTH TO  
NEXT ADJ LOW FLUTE IF AB'S  
ARE LESS THAN 2" FROM  
STRUT  $\bar{r}$  SUPPORT SCREWS  
LENGTH SHALL  
ENGAGE  
2 LOW FLUTES MIN

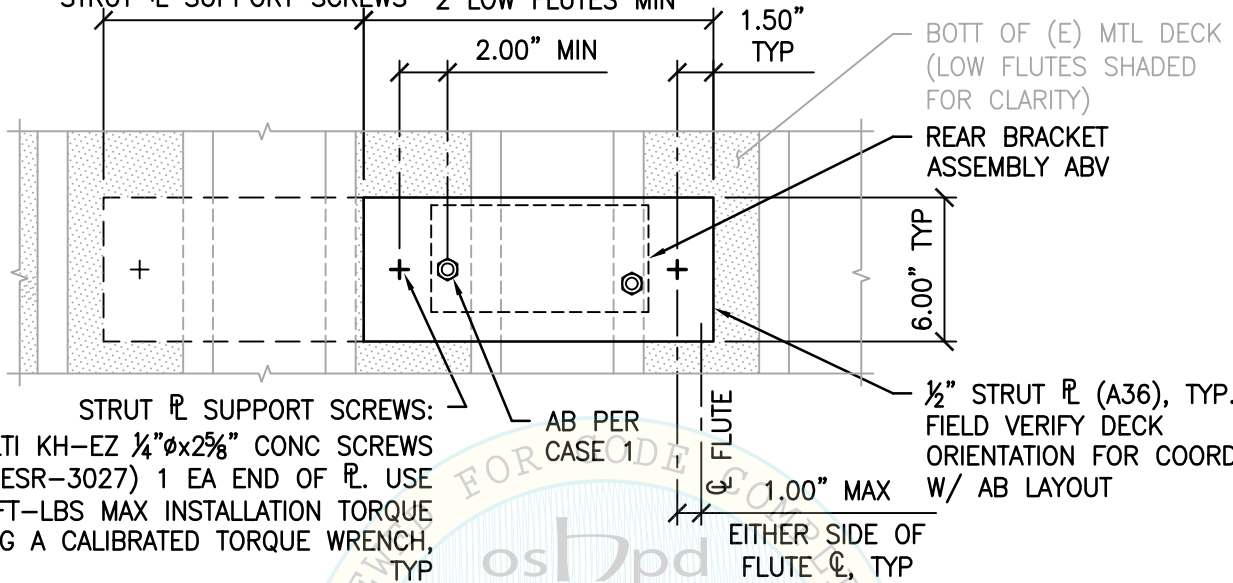

STRUT  $\bar{r}$  SUPPORT SCREWS:  
HILTI KH-EZ  $\frac{1}{4}$ " $\phi$  $\times$  $\frac{5}{8}$ " CONC SCREWS  
(ICC ESR-3027) 1 EA END OF  $\bar{r}$ . USE  
18 FT-LBS MAX INSTALLATION TORQUE  
USING A CALIBRATED TORQUE WRENCH,  
TYP

AB PER  
CASE 1

BOTT OF (E) MTL DECK  
(LOW FLUTES SHADED  
FOR CLARITY)  
REAR BRACKET  
ASSEMBLY ABV

$\frac{1}{2}$ " STRUT  $\bar{r}$  (A36), TYP.  
FIELD VERIFY DECK  
ORIENTATION FOR COORD  
W/ AB LAYOUT


EITHER SIDE OF  
FLUTE  $\bar{c}$ , TYP

**PLAN VIEW**

ANCHORS PERPENDICULAR TO FLUTES

EXTEND STRUT LENGTH TO  
NEXT ADJ LOW FLUTE IF AB'S  
ARE LESS THAN 2" FROM  
STRUT  $\bar{r}$  SUPPORT SCREWS

LENGTH SHALL ENGAGE  
2 LOW FLUTES MIN

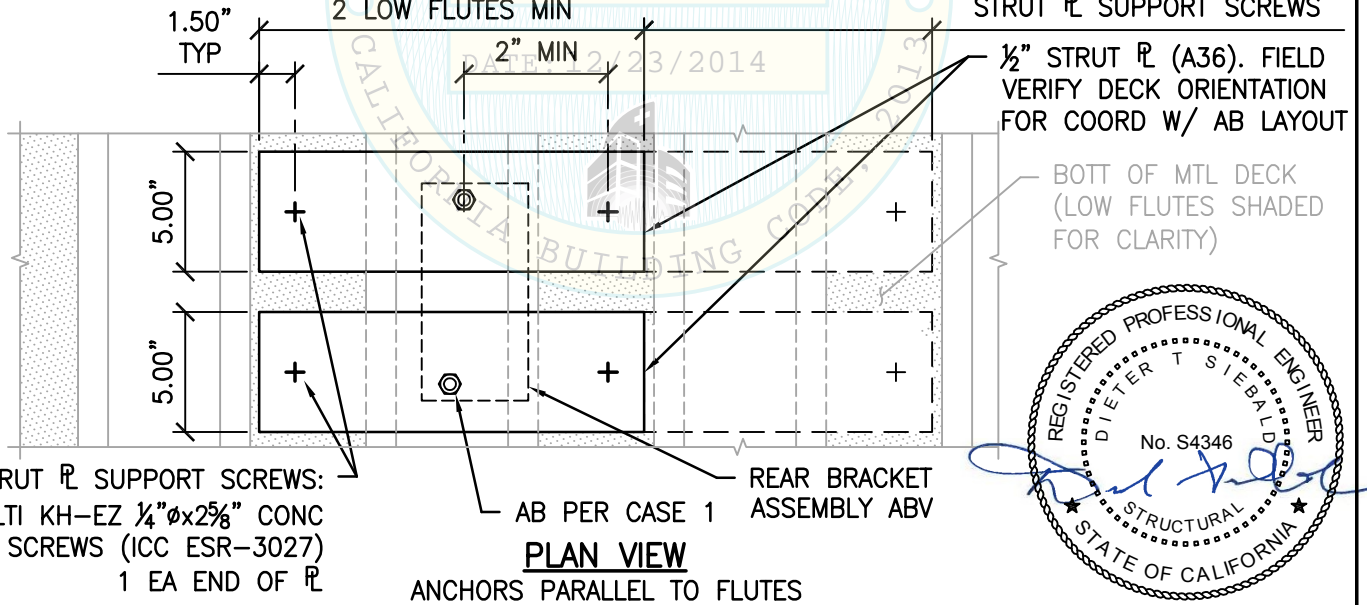

STRUT  $\bar{r}$  SUPPORT SCREWS:  
HILTI KH-EZ  $\frac{1}{4}$ " $\phi$  $\times$  $\frac{5}{8}$ " CONC  
SCREWS (ICC ESR-3027)  
1 EA END OF  $\bar{r}$

**PLAN VIEW**

ANCHORS PARALLEL TO FLUTES

$\frac{1}{2}$ " STRUT  $\bar{r}$  (A36). FIELD  
VERIFY DECK ORIENTATION  
FOR COORD W/ AB LAYOUT

BOTT OF MTL DECK  
(LOW FLUTES SHADED  
FOR CLARITY)



SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE FILL OVER METAL DECK



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	16 of 18



L:\Jobs\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec19,2014-05:33pm Login:camachom Dimscdle:1 L1Scale:6



MAX ANCHOR FORCES AT LRFD AT EACH ANCHOR BOLT

	FRONT BRACKET		REAR BRACKET	
	Tu	Vu	Tu	Vu
CASE 2 z/h=0	1343#	457#	1463#	340#

INCLUDES OVERSTRENGTH FACTOR ( $\Omega_o$ )

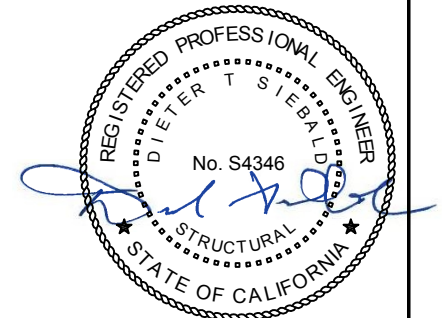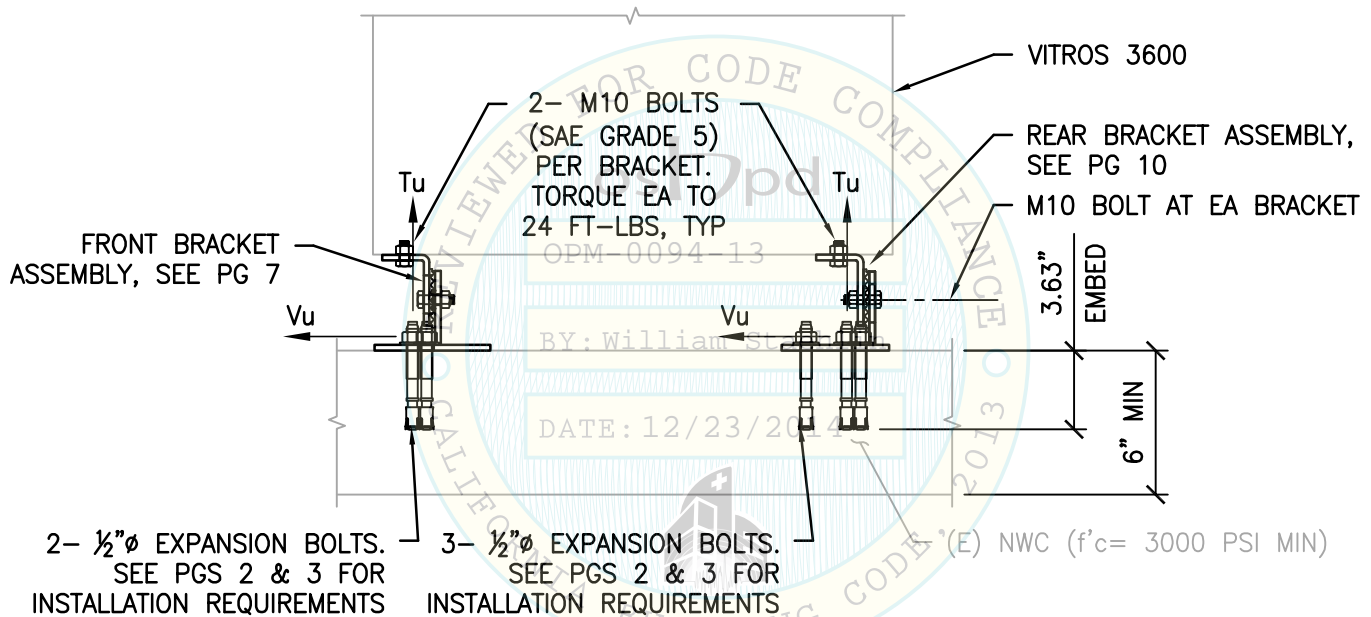

SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE SLAB



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833


TEL (916) 920-2020  
www.cyseng.com

Job No: 13072.02  
Date: 12/19/2014  
Page: 17 of 18

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec19,2014-05:33pm Login:camachom Dimstyle:1 LTScale:6


MAX ANCHOR FORCES AT LRFD AT EACH ANCHOR BOLT				
CASE 3 z/h=0	FRONT BRACKET		REAR BRACKET	
	Tu	Vu	Tu	Vu
	1137#	420#	1290#	316#

INCLUDES OVERSTRENGTH FACTOR ( $\Omega_o$ )

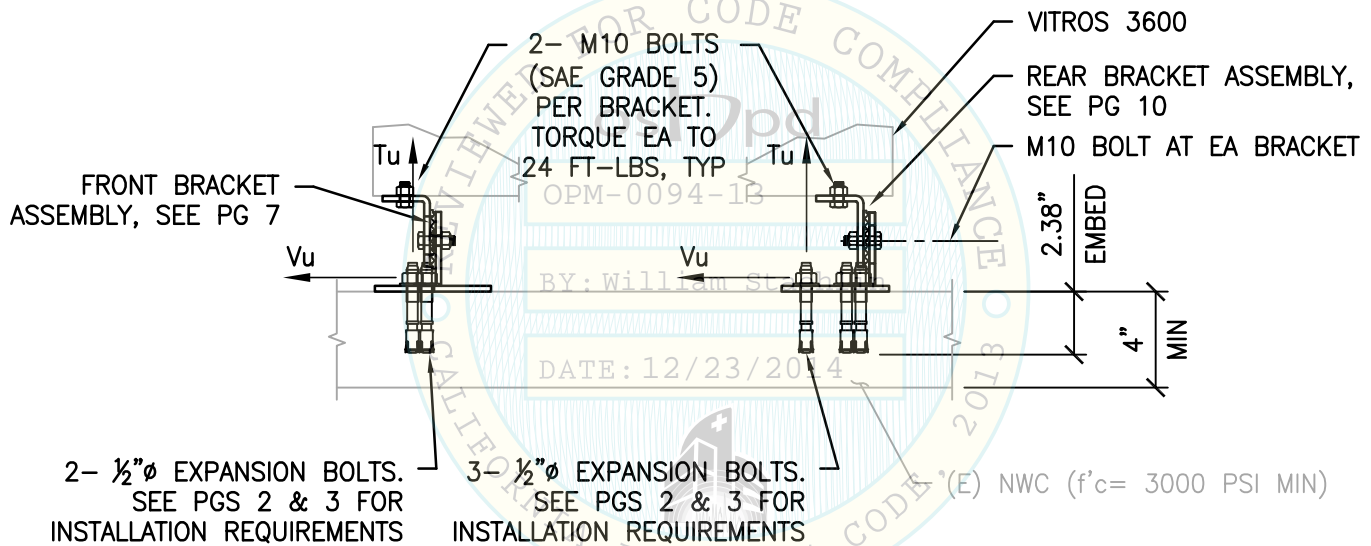

**NOTE:**

THIS ANCHORAGE DETAIL CAN ONLY BE USED AT GEOGRAPHICAL LOCATIONS WHERE  $S_{DS}$  IS LESS THAN OR EQUAL TO 2.30.

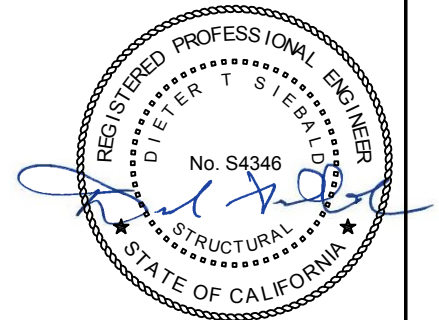

SHEET TITLE: ATTACHMENT DETAIL  
TO CONCRETE SLAB



**CYS STRUCTURAL ENGINEERS, INC.**

2495 NATOMAS PARK DRIVE, SUITE 650  
SACRAMENTO, CA 95833

TEL (916) 920-2020  
www.cyseng.com

Job No:	13072.02
Date:	12/19/2014
Page:	18 of 18

L:\Jobs\13\13072 OCDUS - Six OPMs\Task 02 - OPM-0094-13 Vitros 3600\STRU\S1\_TASK 02.dwg Time:Dec 19, 2014 - 05:33pm Login:camachom Dimstyle:1 LTScale:6