



DEPARTMENT OF HEALTH CARE ACCESS AND INFORMATION
OFFICE OF STATEWIDE HOSPITAL PLANNING AND DEVELOPMENT

APPLICATION FOR HCAI PREAPPROVAL OF
MANUFACTURER'S CERTIFICATION (OPM)

OFFICE USE ONLY

APPLICATION #: OPM-0746

HCAI Preapproval of Manufacturer's Certification (OPM)

Type: ☒ New ☐ Renewal/Update

Manufacturer Information

Manufacturer: Beckman Coulter, Inc

Manufacturer's Technical Representative: Sam Rizzotte

Mailing Address: 250 S. Kramer Blvd, Brea, CA 928211722

Telephone: (657) 286-3667

Email: shrizzotte@beckman.com

Product Information

Product Name: Power Link Workcell

Product Type: Other electrical and mechanical components

Product Model Number: 9720, 9722, 9V04

General Description: Connects chemical analyzers AU680 or Dxc700 to the Dxl 800 or Dxl 600 immunoassay analyzers for improved efficiency.

Applicant Information

Applicant Company Name: EASE LLC.

Contact Person: Tiffany Tonn

Mailing Address: 1515 FAIRVIEW AVE, STE 205, MISSOULA, MT 59801

Telephone: (406) 541-3273

Email: tiffany@easeco.com

Title: Office Assistant

"A healthier California where all receive equitable, affordable, and quality health care"

STATE OF CALIFORNIA – HEALTH AND HUMAN SERVICES AGENCY





DEPARTMENT OF HEALTH CARE ACCESS AND INFORMATION
OFFICE OF STATEWIDE HOSPITAL PLANNING AND DEVELOPMENT

Registered Design Professional Preparing Engineering Recommendations

Company Name: EASE LLC

Name: Jonathan Roberson

California License Number: S4197

Mailing Address: 5877 Pine Ave., Suite 210, Chino Hills, CA 91709

Telephone: (951) 295-1892

Email: jon@EASECo.com

HCAI Special Seismic Certification Preapproval (OSP)

☐ Special Seismic Certification is preapproved under OSP

OSP Number: _____

Certification Method

Testing in accordance with: ☐ ICC-ES AC156 ☐ FM 1950-16

☐ Other(s) (Please Specify): _____

*Use of criteria other than those adopted by the California Building Standards Code, 2022 (CBSC 2022) for component supports and attachments are not permitted. For distribution system, interior partition wall, and suspended ceiling seismic bracings, test criteria other than those adopted in the CBSC 2022 may be used when approved by HCAI prior to testing.

☒ Analysis

☐ Experience Data

☐ Combination of Testing, Analysis, and/or Experience Data (Please Specify): _____

HCAI Approval

Date: 1/20/2025

Name: William Staehlin

Title: Senior Structural Engineer

Condition of Approval (if applicable): _____

"A healthier California where all receive equitable, affordable, and quality health care"

STATE OF CALIFORNIA – HEALTH AND HUMAN SERVICES AGENCY





**EQUIPMENT ANCHORAGE
& SEISMIC ENGINEERING**

5877 Pine Ave, Ste. 210
Chino Hills, CA. 91709
Phn: (909) 606-7622

The Department of Health Care Access and Information
PREAPPROVAL OF MANUFACTURER'S CERTIFICATION
OPM-0746

THIS PREAPPROVAL CONFORMS TO THE 2022 CALIFORNIA BUILDING CODE

MANUFACTURER: **BECKMAN COULTER**
EQUIPMENT NAME: **POWERLINK**

Sheet: 1 of 20

Date: 1/16/25

GENERAL NOTES

1. THIS HCAI PREAPPROVAL OF MANUFACTURER'S CERTIFICATION (OPM) IS BASED ON THE 2022 CBC. THE DEMANDS (DESIGN FORCES) FOR USE WITH THIS OPM SHALL BE BASED ON THE 2022 CBC
2. THIS DOCUMENT MAY ONLY BE USED WITH THE EXPRESS WRITTEN CONSENT OF THE MANUFACTURER LISTED ABOVE FOR THE SPECIFIC PROJECT SITE AND INSTALLATION LOCATION. THIS DOCUMENT IS INVALID WITHOUT SUCH CONSENT.
3. THIS PREAPPROVAL CONFORMS TO THE 2022 CALIFORNIA BUILDING CODE WHERE S_{ds} IS NOT GREATER THAN 2.5.
4. FORCES PER ASCE 7-16 SECTION 13.3.1, EQUATIONS 13.3-1, 13.3-2 & 13.3-3, WHERE $S_{ds} = 2.30$, $a_p = 1.0$, $I_p = 1.5$, $R_p = 1.5$, $z/h = 0$ AT CONCRETE SLAB & $z/h \leq 1$ AT CONCRETE SLAB ON METAL DECK. SEE FOLLOWING SHEETS FOR Ω_o .
5. THIS PREAPPROVAL COVERS ONLY THE SUPPORTS AND ATTACHMENTS OF THE EQUIPMENT TO THE STRUCTURE.
6. ALL DESIGN FORCES SHOWN ON THE DRAWINGS ARE FACTORED LOADS THAT SHALL BE USED FOR STRENGTH DESIGN.
7. CONCRETE SLAB ON METAL DECK DETAIL VALID FOR DEMANDS SHOWN AT ANY ELEVATION IN THE BUILDING. (i.e. $z/h \leq 1$)
8. CONCRETE SLAB DETAIL VALID FOR DEMANDS SHOWN AT OR BELOW GRADE. (i.e. $z/h = 0$)
9. **RESPONSIBILITIES OF THE STRUCTURAL ENGINEER OF RECORD OF THE BUILDING**
 - A. PROVIDE SUPPORTING STRUCTURE TO SUPPORT WEIGHTS AND FORCES SHOWN IN ADDITION TO ALL OTHER LOADS.
 - B. VERIFY THAT THE INSTALLATION IS IN CONFORMANCE WITH THE 2022 CBC AND WITH THE DETAILS, MATERIAL AND GAGE OF THE UNIT WHERE ATTACHMENTS ARE MADE AGREE WITH THE INFORMATION SHOWN ON THE PREAPPROVAL DOCUMENTS.
 - C. VERIFY THAT PROJECT SPECIFIC VALUES OF S_{ds} & z/h RESULT IN SEISMIC FORCES (E_h , E_v) THAT DO NOT EXCEED THE VALUES ON THE DETAILS.
 - D. VERIFY THAT THE CONCRETE SLAB TO WHICH THE EQUIPMENT IS ANCHORED MEETS THE REQUIREMENTS OF THE APPLICABLE ICC ESR REPORT AND THIS OPM.
 - E. VERIFY THAT THE ANCHORS ARE AN ADEQUATE DISTANCE FROM ANY SLAB EDGES OR OPENINGS (SEE TYPICAL DETAIL ON SHEET 2).
 - F. VERIFY THAT ALL NEW OR EXISTING ANCHORS ARE AN ADEQUATE DISTANCE FROM THE UNIT ATTACHMENTS AND CHECK FOR INTERACTION WHERE OTHER ANCHORS ARE WITHIN 18" OR $6h_{ef}$ FROM THIS UNIT'S ANCHORS.



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET

2

OF 20 SHEETS

10. EXPANSION ANCHORS:

- A. ATTACHMENT IS TO BE MADE WITH THE ANCHORS LISTED BELOW AND INSTALLED AS DESCRIBED IN THE CORRESPONDING ICC REPORT.

Anchor Diameter	Concrete Type	Min. f _c (psi)	Anchor Type	ICC Report No.	Min. Embed.	Min. Spacing	Min. Edge Dist.	Min. Conc. Thickness	Torque Test	Direct Tension Test
1/2"	Sand Light Weight	3000	Hilti Kwik Bolt TZ2 (CARBON STEEL)	ESR-4266	2.5"	6.75"	12"	See Detail "A"	50 FT-LB	N/A
5/8"	Normal Weight	3000	Hilti Kwik Bolt TZ2 (CARBON STEEL)	ESR-4266	3.25"	4"	32"	6"	40 FT-LB	2895 lb

- B. THIS PREAPPROVAL ALLOWS FOR UP TO A MAXIMUM OF 2 ADJACENT CONCRETE SLAB EDGES, 32" AWAY MINIMUM (i.e. - CORNER). SEE ADJACENT DETAIL FOR ADDITIONAL MINIMUM ALLOWABLE CONCRETE EDGE DISTANCES.

- C. TESTING AND SPECIAL INSPECTION OF EXPANSION ANCHORS SHALL BE PERFORMED BY AN APPROVED INDEPENDENT AGENCY EMPLOYED BY THE FACILITY OWNER PER CBC 1704A & 1910A.5 AND CAC 7-149. ALL REPORTS SHALL BE SENT TO THE INSPECTOR OF RECORD, OWNER AND THE ARCHITECT OR ENGINEER IN RESPONSIBLE CHARGE.

- (i) AFTER AT LEAST 24 HOURS HAVE ELAPSED SINCE INSTALLATION, DIRECT PULL TENSION TEST OR TORQUE TEST AT LEAST 50% OF THE ANCHORS.

- (ii) ACCEPTANCE CRITERIA:

- DIRECT TENSION TEST: THE ANCHOR SHOULD HAVE NO OBSERVABLE MOVEMENT AT THE TEST LOAD. A PRACTICAL WAY TO DETERMINE OBSERVABLE MOVEMENT IS THAT THE WASHER BECOMES LOOSE.
- TORQUE TEST: THE APPLICABLE TORQUE MUST BE ACHIEVED WITHIN THE FOLLOWING LIMITS: WEDGE TYPE : 1/2 TURN OF THE NUT


- (iii) IF ANY ANCHOR FAILS, TEST ALL ANCHORS.

- D. AVOID DAMAGING EXISTING STEEL REINFORCING IN CONCRETE SLAB WHEN INSTALLING CONCRETE EXPANSION ANCHORS.


- E. PROVIDE FOR FULL THREAD ENGAGEMENT OF NUT & WASHER.

11. BOLTS THROUGH CONCRETE ON METAL DECK

- A. BOLTS SHALL BE TORQUED BY 3/4 TURN OF THE NUTS AFTER THE SNUG TIGHT (THE SNUG-TIGHT CONDITION IS DEFINED AS THE TIGHTNESS REQUIRED TO BRING THE CONNECTED PLIES INTO FIRM CONTACT) CONDITION IS ACHIEVED, UNLESS OTHERWISE NOTED.
- B. THROUGH BOLT HOLES SHALL BE 1/16" LARGER THAN BOLT SIZE (HOLE SIZE = BOLT SIZE + 1/16) FOR CONCRETE.
- C. THROUGH-BOLTS IN CONCRETE SHALL RECEIVE SPECIAL INSPECTION AND TESTING (THROUGH BOLTS WITH STEEL TO STEEL CONNECTION IN TENSION DO NOT REQUIRE TENSION TESTING) IN ACCORDANCE WITH REQUIREMENTS FOR POST-INSTALLED ANCHORS.

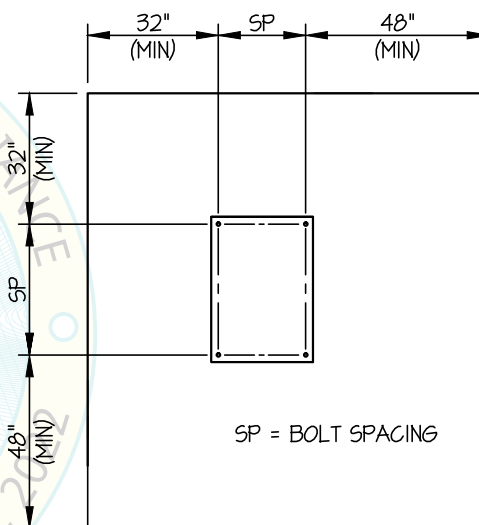

TYPICAL CONCRETE EDGE DETAIL
(SLAB ON GRADE ONLY)

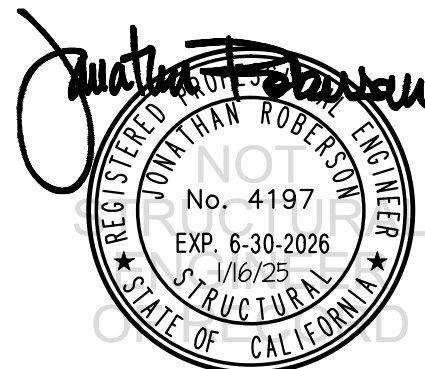

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


3

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE I

CONCRETE SLAB

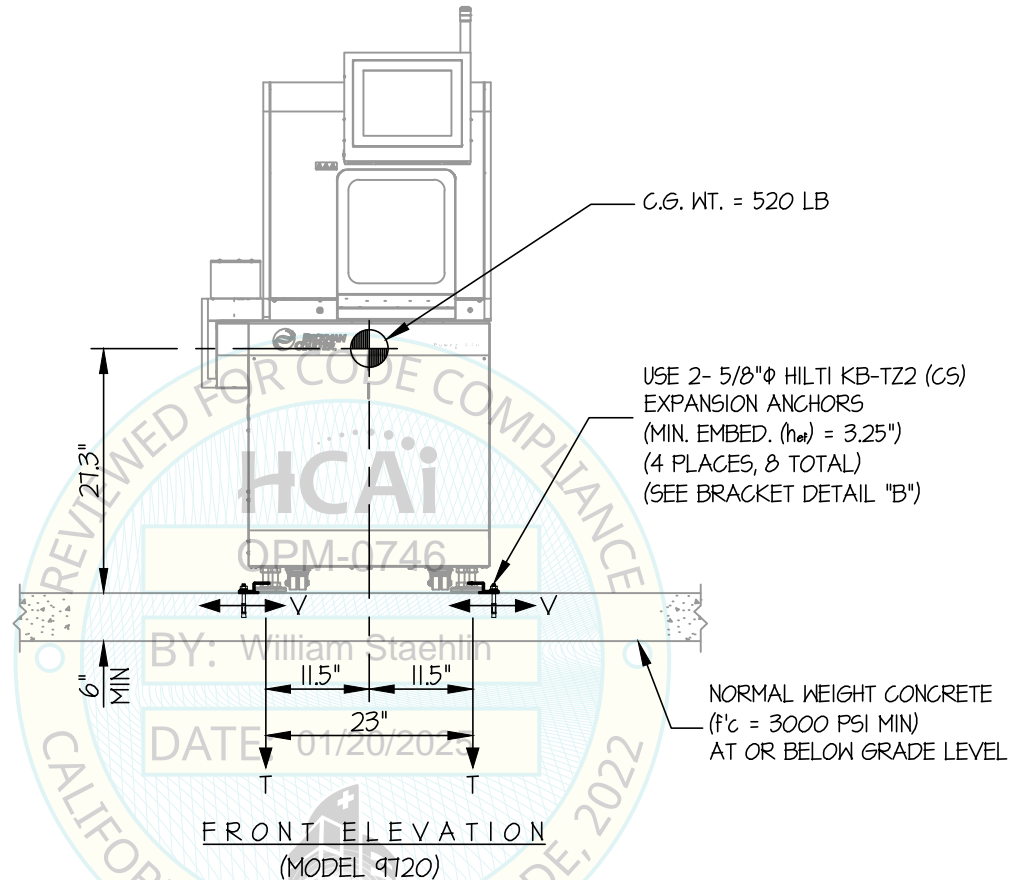


$T_U = 1426$ LB/BOLT (MAX)
 $V_U = 955$ LB/BOLT (MAX)
 (VALUES INCLUDE Ω)

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: $S_{ds} = 2.30$, $a_p = 1.0$, $I_p = 1.5$, $R_p = 1.5$, $\Omega_o = 2.0$, $z/h = 0$)

HORIZONTAL FORCE (E_h) = 1.035 W_p
 HORIZONTAL FORCE (E_{mh}) = 2.07 W_p (FOR CONCRETE ANCHORAGE)
 VERTICAL FORCE (E_v) = 0.46 W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2

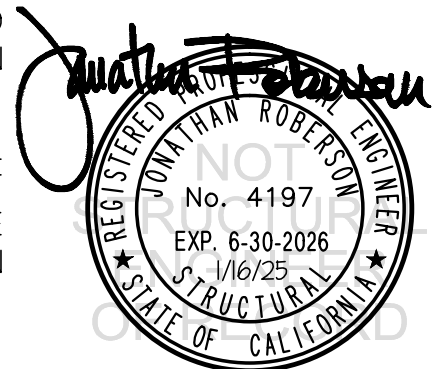

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET

4

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 1




CONCRETE SLAB

C.G. WT. = 520 LB
(\bar{Y} = 27.3")

USE 2- 5/8" Φ HILTI KB-TZ2 (CS)
EXPANSION ANCHORS
(MIN. EMBED. (h_{ef}) = 3.25")
(4 PLACES, 8 TOTAL)
(SEE BRACKET DETAIL "B")

BY: William Staehlin

PLAN AT BASE
DATE: (MODEL 9720) 25

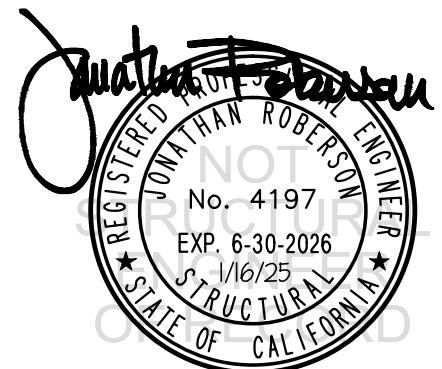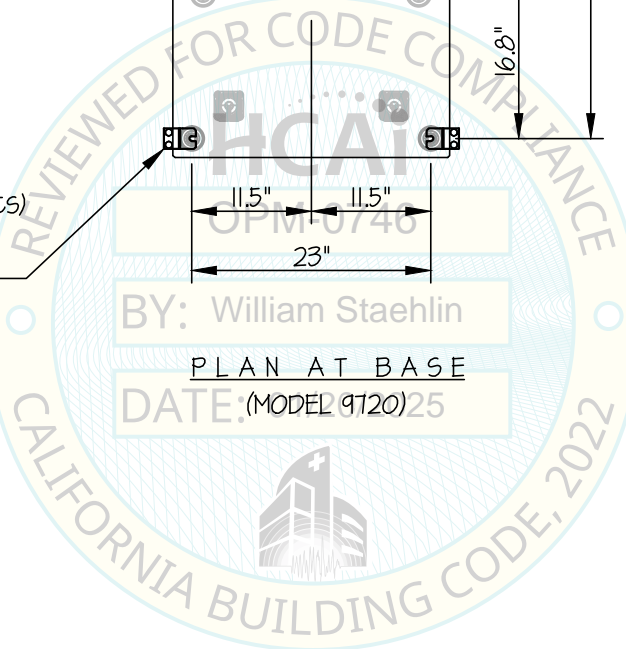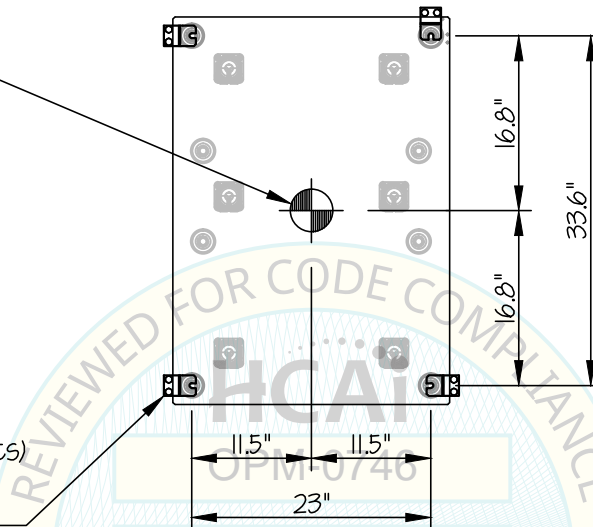

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


5

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 2

CONCRETE SLAB

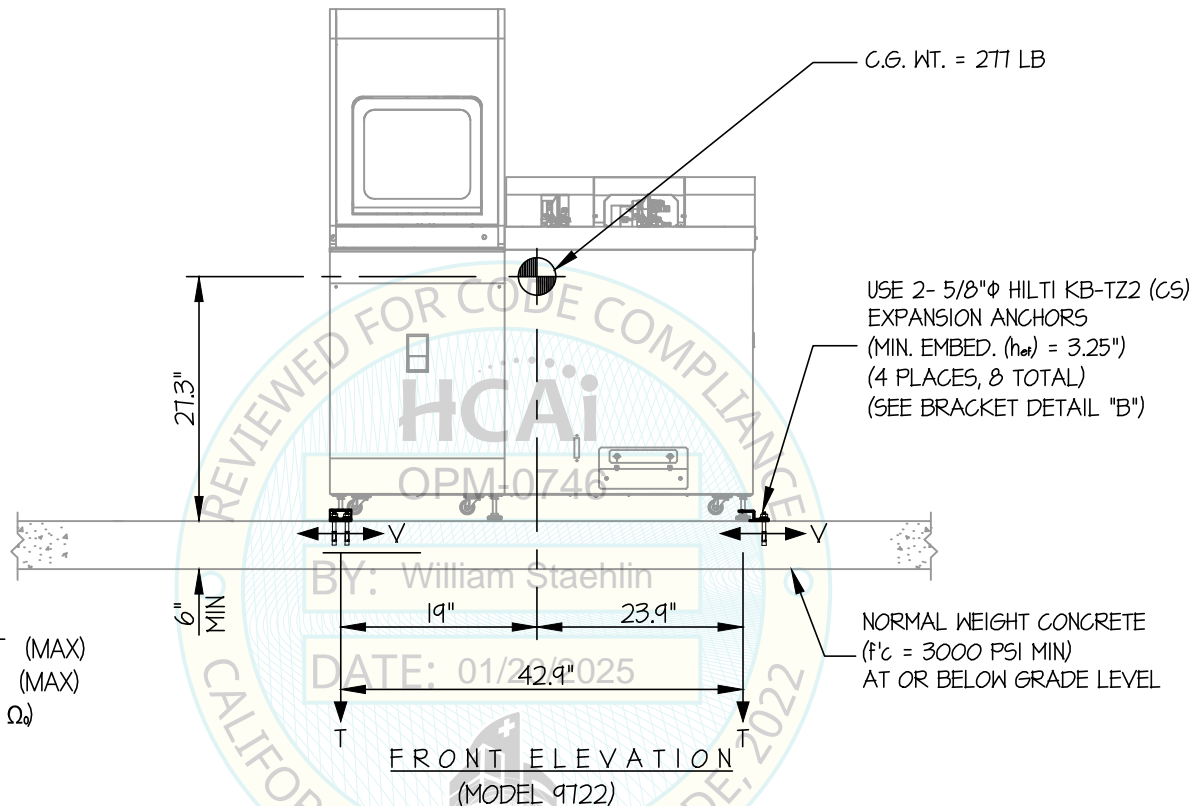

T_u = 1778 LB/BOLT (MAX)
 V_u = 544 LB/BOLT (MAX)
 (VALUES INCLUDE Ω)

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: S_{DS} = 2.30, a_p = 10, I_p = 15, R_p = 15, Ω_o = 2.0, z/h = 0)
 HORIZONTAL FORCE (E_h) = 1.035 W_p
 HORIZONTAL FORCE (E_{mh}) = 2.07 W_p (FOR CONCRETE ANCHORAGE)
 VERTICAL FORCE (E_v) = 0.46 W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET



6

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 2

CONCRETE SLAB

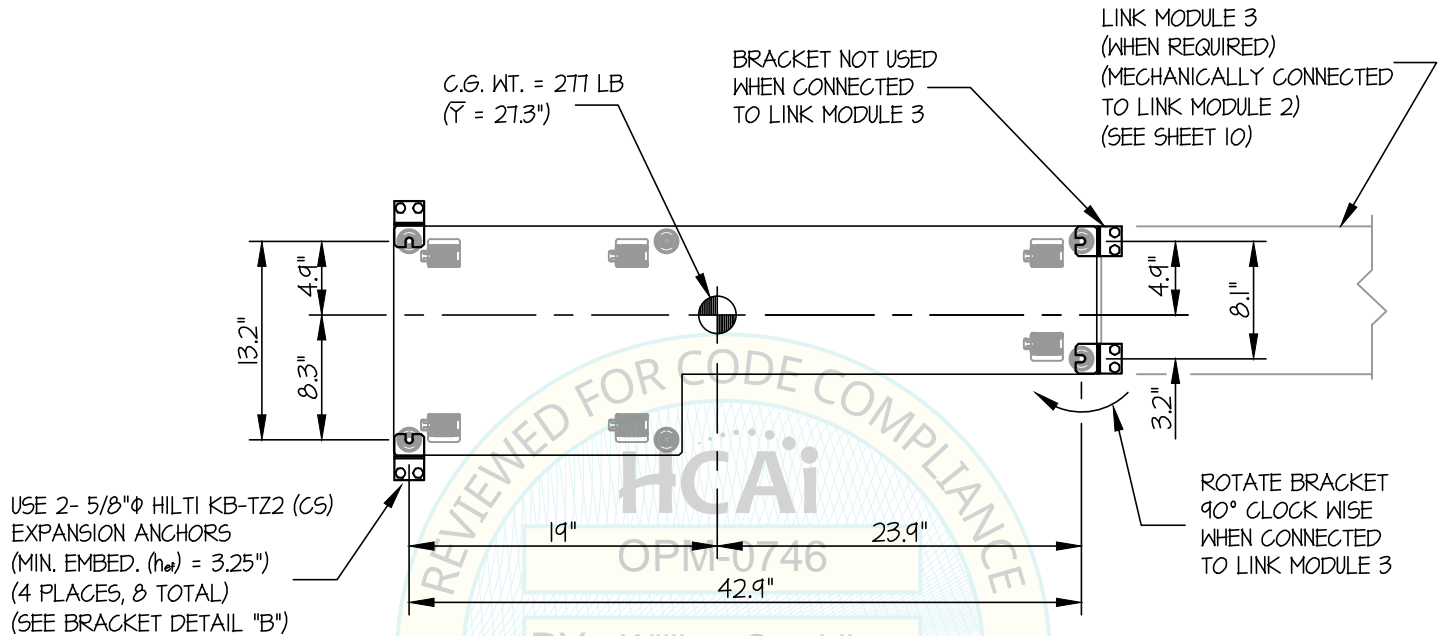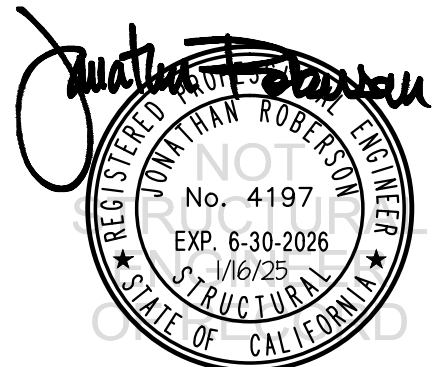BY: William Staehlin
PLAN AT BASE(MODEL 9122)
DATE: 01/20/2025REVIEWED FOR CODE COMPLIANCE
HCAi
OPM-0746
CALIFORNIA BUILDING CODE, 2022

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25


SHEET

7

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

CONCRETE SLAB

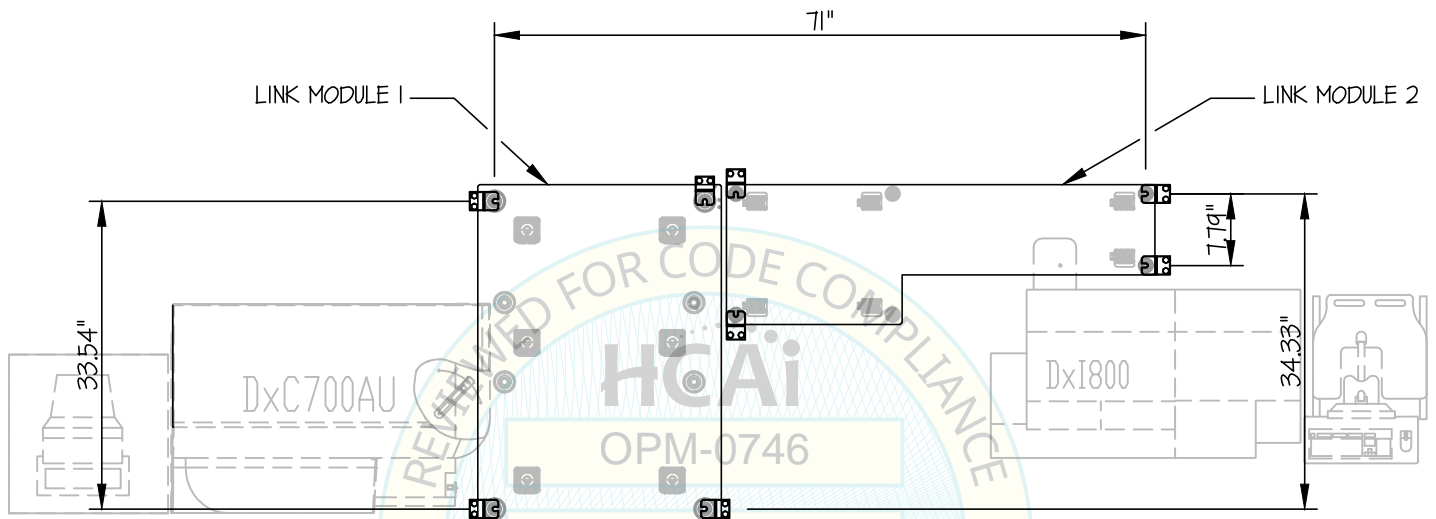

USE 2- 5/8" ϕ HILTI KB-TZ2 (CS)
EXPANSION ANCHORS
(MIN. EMBED. (h_{ef}) = 3.25")
(8 PLACES, 16 TOTAL)
(SEE BRACKET DETAIL "B")

LAYOUT
90HS (9720+9722)



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


8

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 3

CONCRETE SLAB

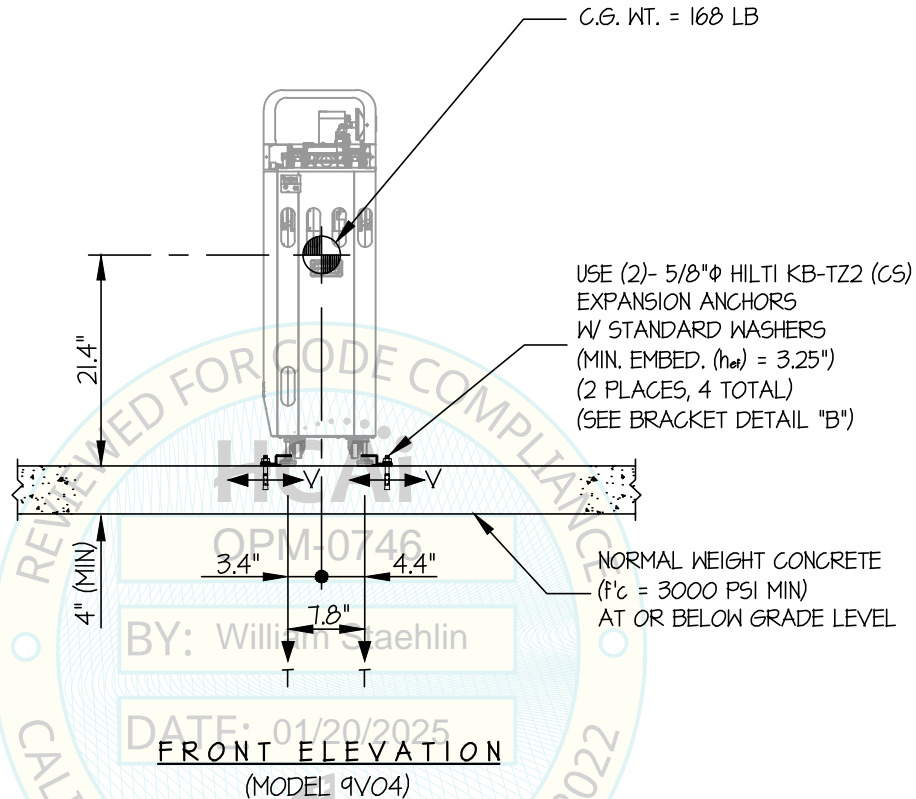 $T_u = 1007$ LB/BOLT (MAX) $V_u = 235$ LB/BOLT (MAX)

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: $S_{ds} = 2.30$, $a_p = 10$, $I_p = 1.5$, $R_p = 1.5$, $\Omega_o = 2.0$, $z/h = 0$)

HORIZONTAL FORCE (E_h)	= 1.035	W_p
HORIZONTAL FORCE (E_{mh})	= 2.07	W_p (FOR CONCRETE ANCHORAGE)
VERTICAL FORCE (E_v)	= 0.46	W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET



9

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 3

CONCRETE SLAB

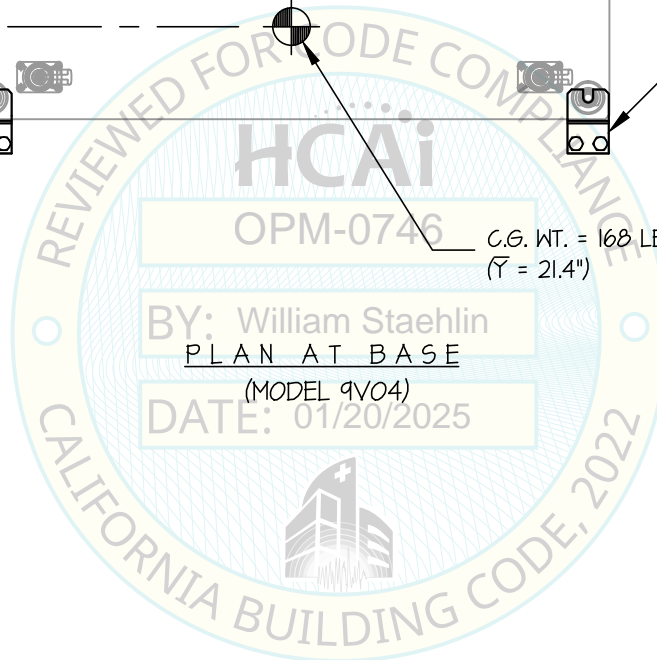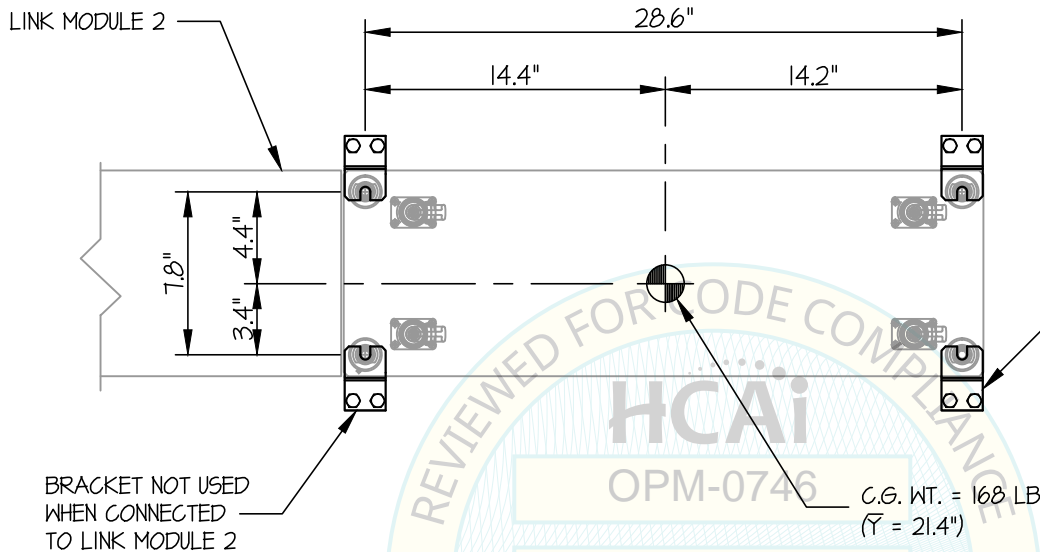

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET



10

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

CONCRETE SLAB

LINK MODULE 3
(WHEN REQUIRED)
(MECHANICALLY CONNECTED AT TRACK
TO LINK MODULE 2 W/ (2) M3 (CL 5.8) CAP SCREWS,
CONNECTOR PLATE AND TAPPED BACKING PLATE)
(2 PLACES)

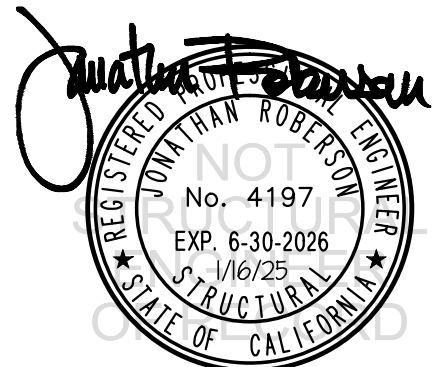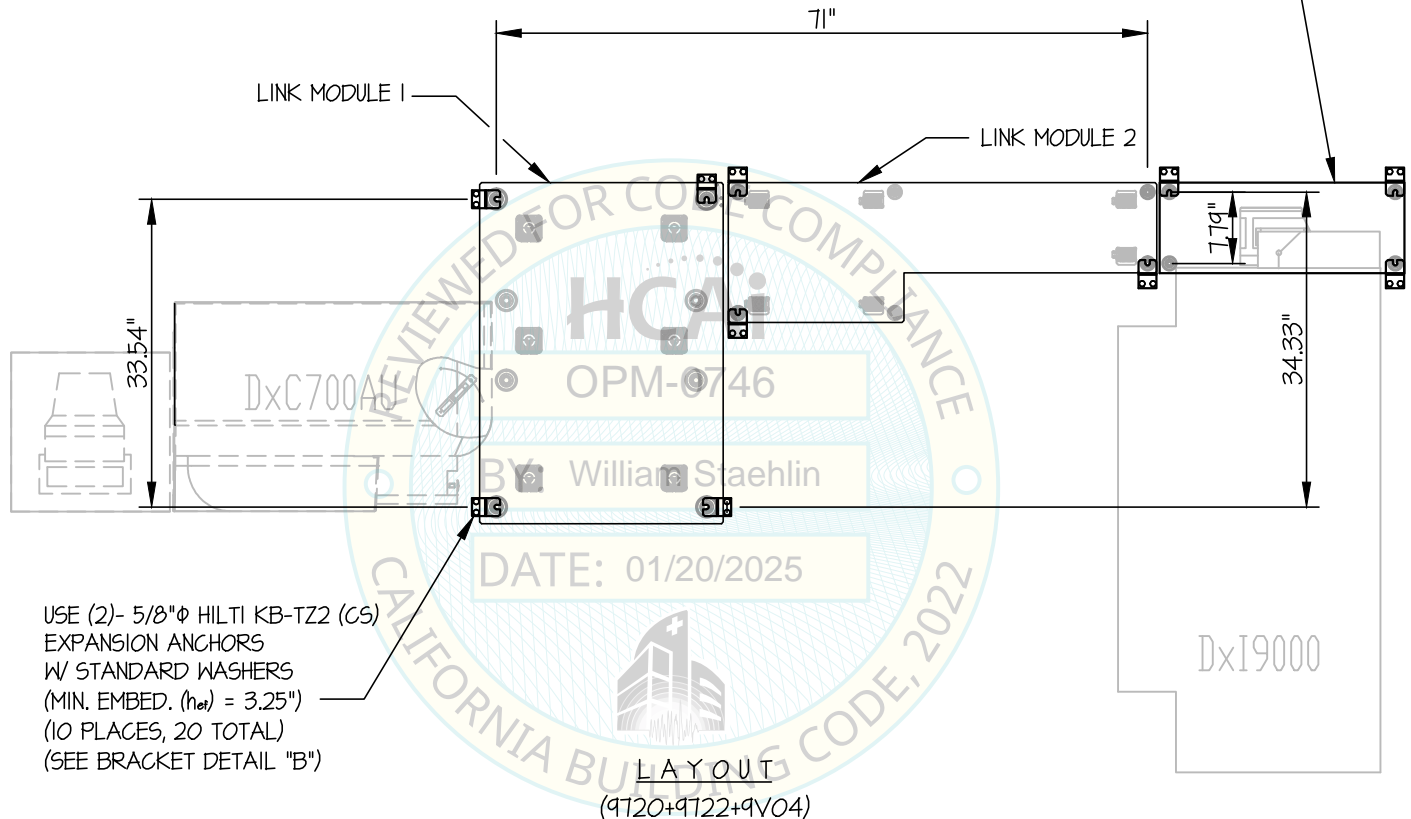

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


11

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE I

CONCRETE SLAB ON METAL DECK

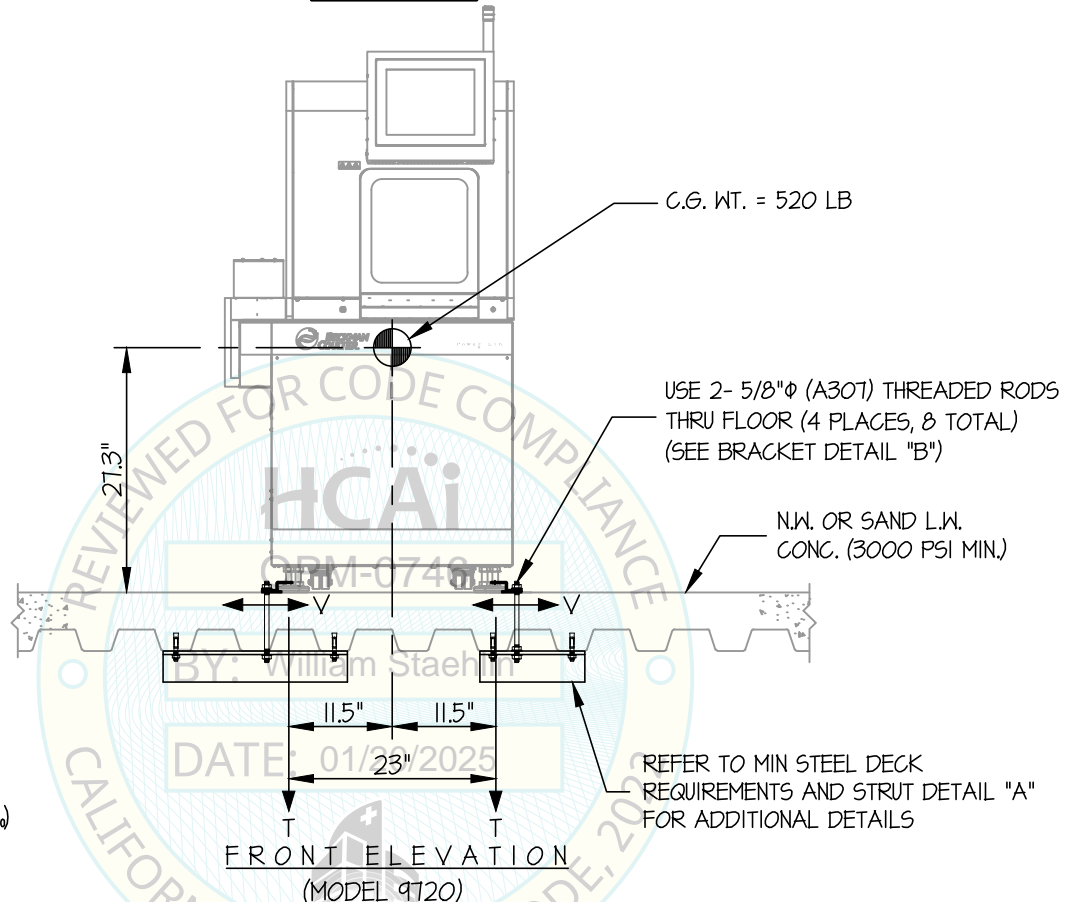

$T_u = 1940$ LB/BOLT (MAX)
 $V_u = 1274$ LB/BOLT (MAX)
 (VALUES DO NOT INCLUDE Ω_u)

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: $S_{ds} = 2.30$, $a_p = 1.0$, $I_p = 1.5$, $R_p = 1.5$, $\Omega_u = 2.0$, $z/h \leq 1$)

HORIZONTAL FORCE (E_h)	= 2.76	W_p
HORIZONTAL FORCE (E_{mh})	= 5.52	W_p (FOR CONCRETE ANCHORAGE)
VERTICAL FORCE (E_v)	= 0.46	W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2



BECKMAN COULTER

DES. J. ROBERSON

SHEET

12

JOB NO. 11-2412

POWERLINK

DATE 1/16/25

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE I


CONCRETE SLAB ON METAL DECK

C.G. WT. = 520 LB
(\bar{Y} = 27.3")

USE 2- 5/8" ϕ (A307) THREADED RODS
THRU FLOOR (4 PLACES, 8 TOTAL)
(SEE BRACKET DETAIL "B")

BY: William Staehlin

PLAN AT BASE
DATE: (MODEL 9720) 25

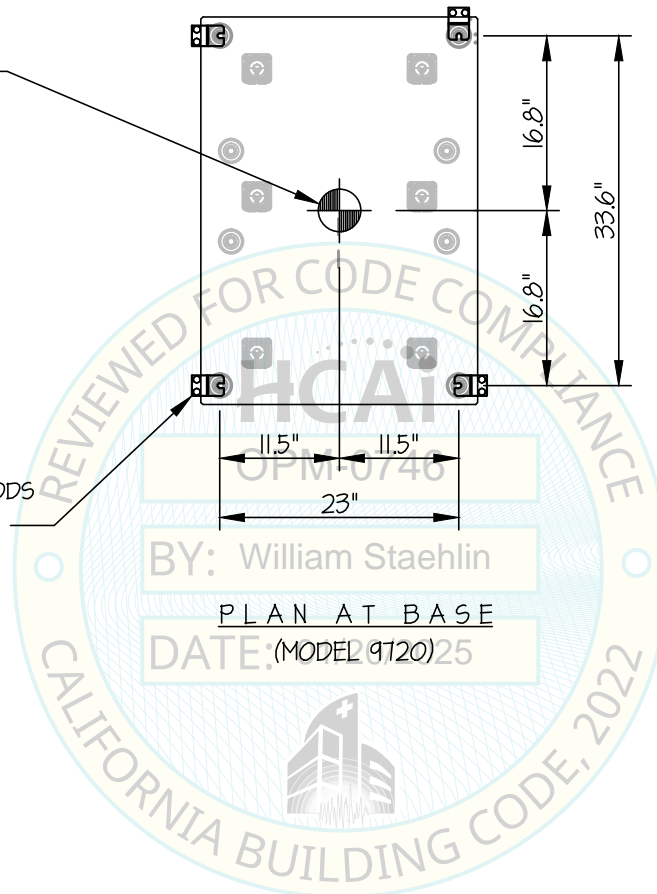

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


13

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 2

CONCRETE SLAB ON METAL DECK

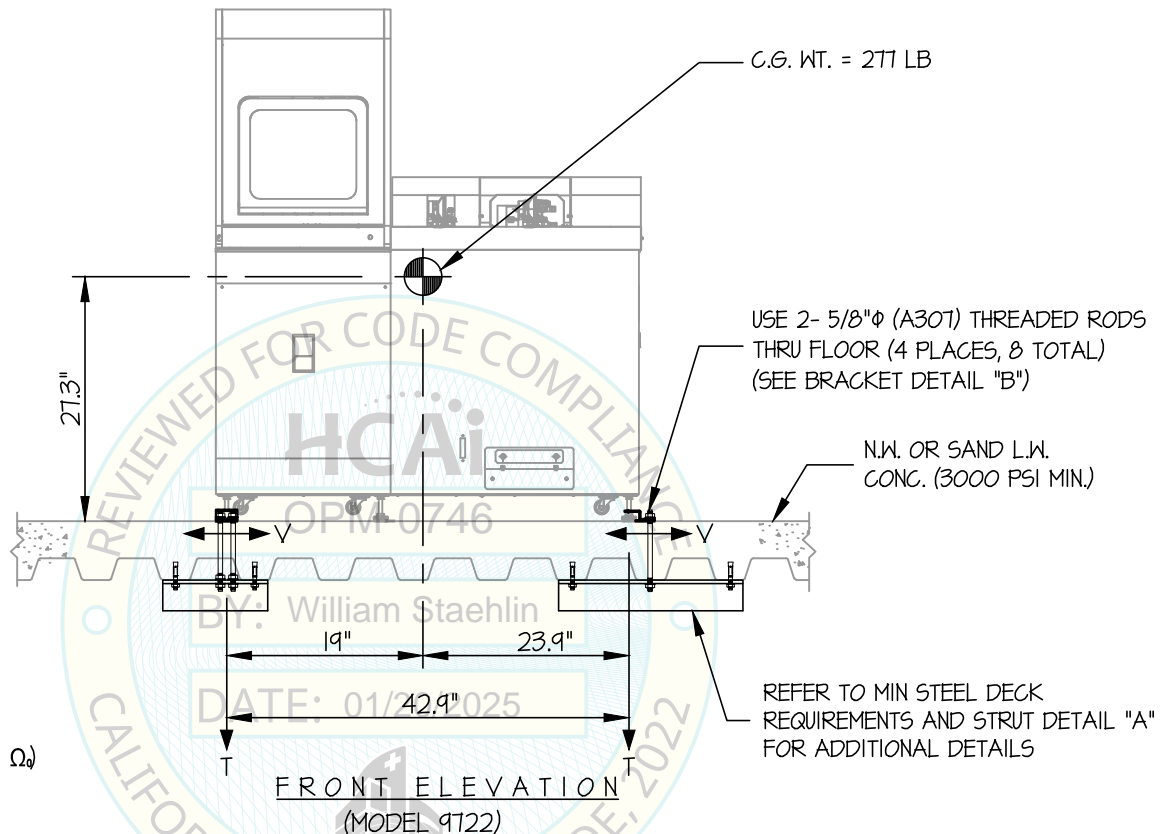

$T_u = 2394$ LB/BOLT (MAX)
 $V_u = 725$ LB/BOLT (MAX)
 (VALUES DO NOT INCLUDE Ω_d)

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: $S_{ds} = 2.30$, $a_p = 1.0$, $I_p = 1.5$, $R_p = 1.5$, $\Omega_o = 2.0$, $z/h \leq 1$)

HORIZONTAL FORCE (E_h)	= 2.76	W_p
HORIZONTAL FORCE (E_{mh})	= 5.52	W_p (FOR CONCRETE ANCHORAGE)
VERTICAL FORCE (E_v)	= 0.46	W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


14

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 2

CONCRETE SLAB ON METAL DECK

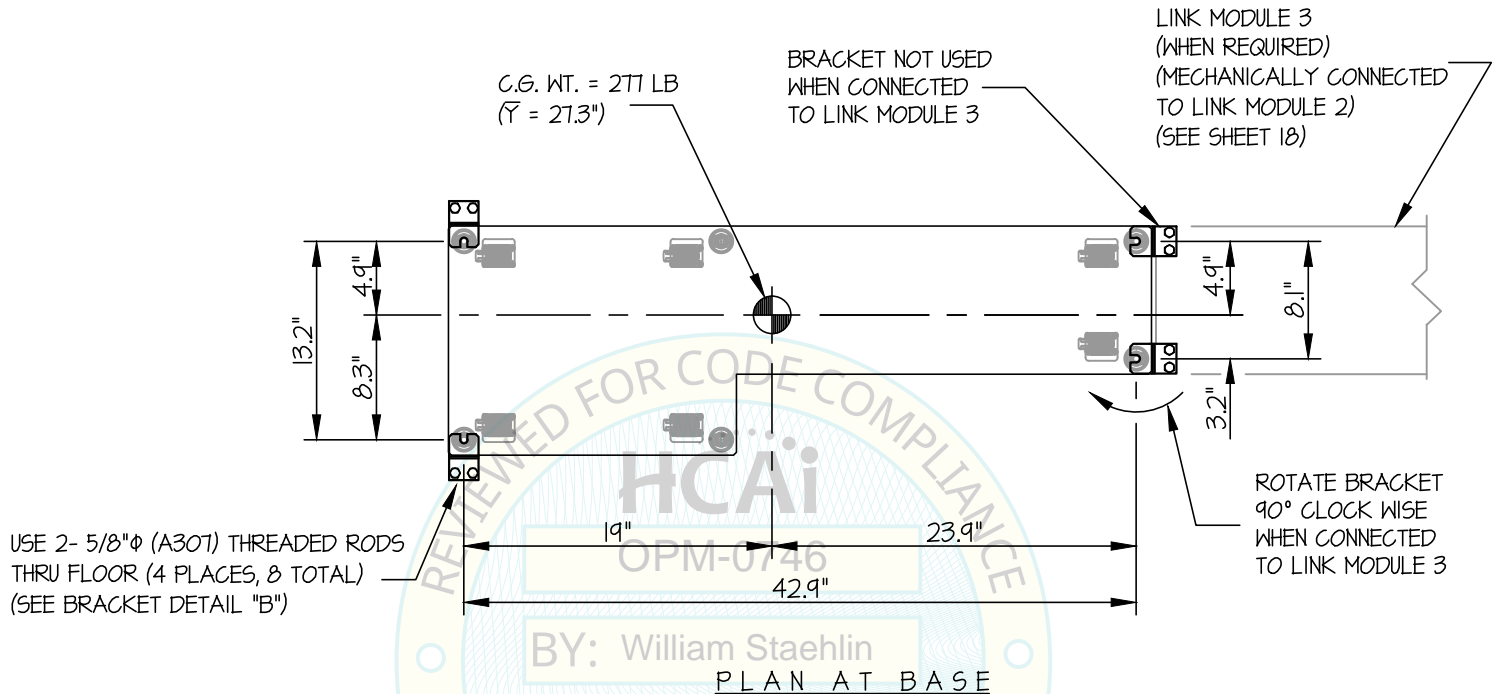

BY: William Staehlin

PLAN AT BASE

(MODEL 9122)

DATE: 01/20/2025



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25


SHEET

15

OF 20 SHEETS


SEISMIC SUPPORTS & ATTACHMENTS

CONCRETE SLAB ON METAL DECK

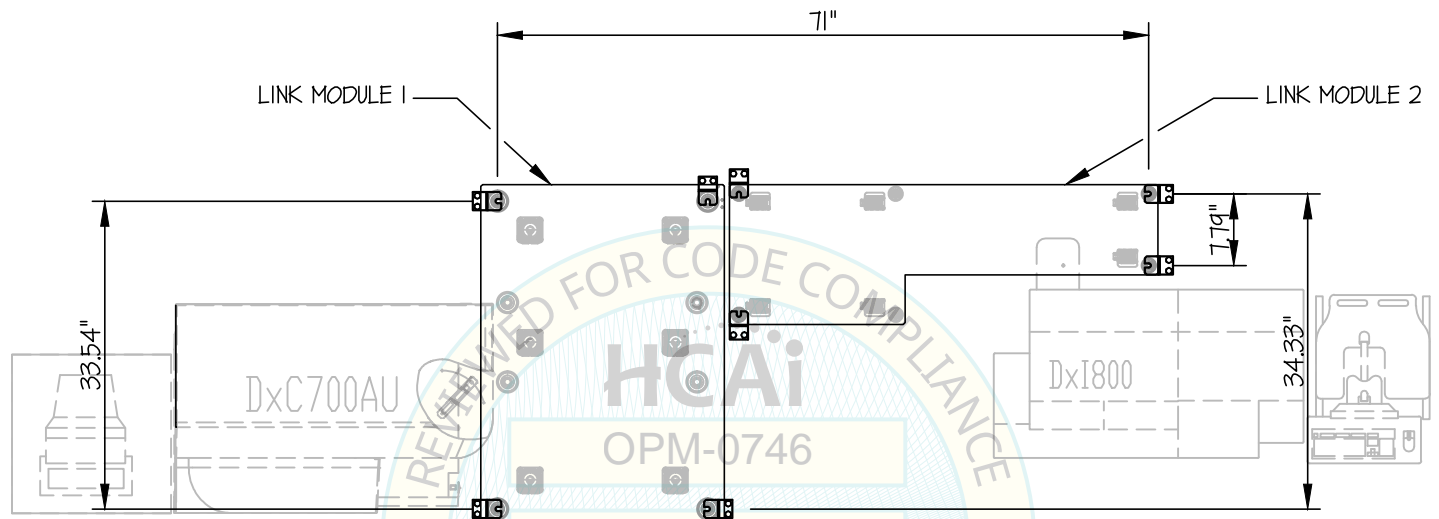

USE 2- 5/8" (A307) THREADED RODS
THRU FLOOR (8 PLACES, 16 TOTAL)
(SEE BRACKET DETAIL "B")

LAYOUT
90HS (9720+9722)

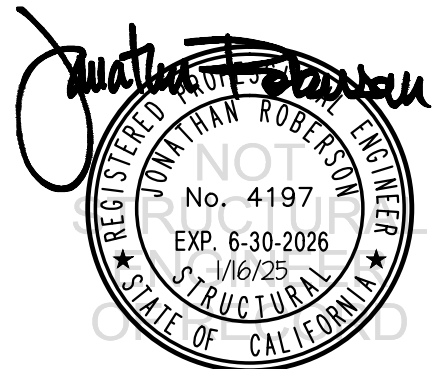

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


16

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 3

CONCRETE SLAB ON METAL DECK

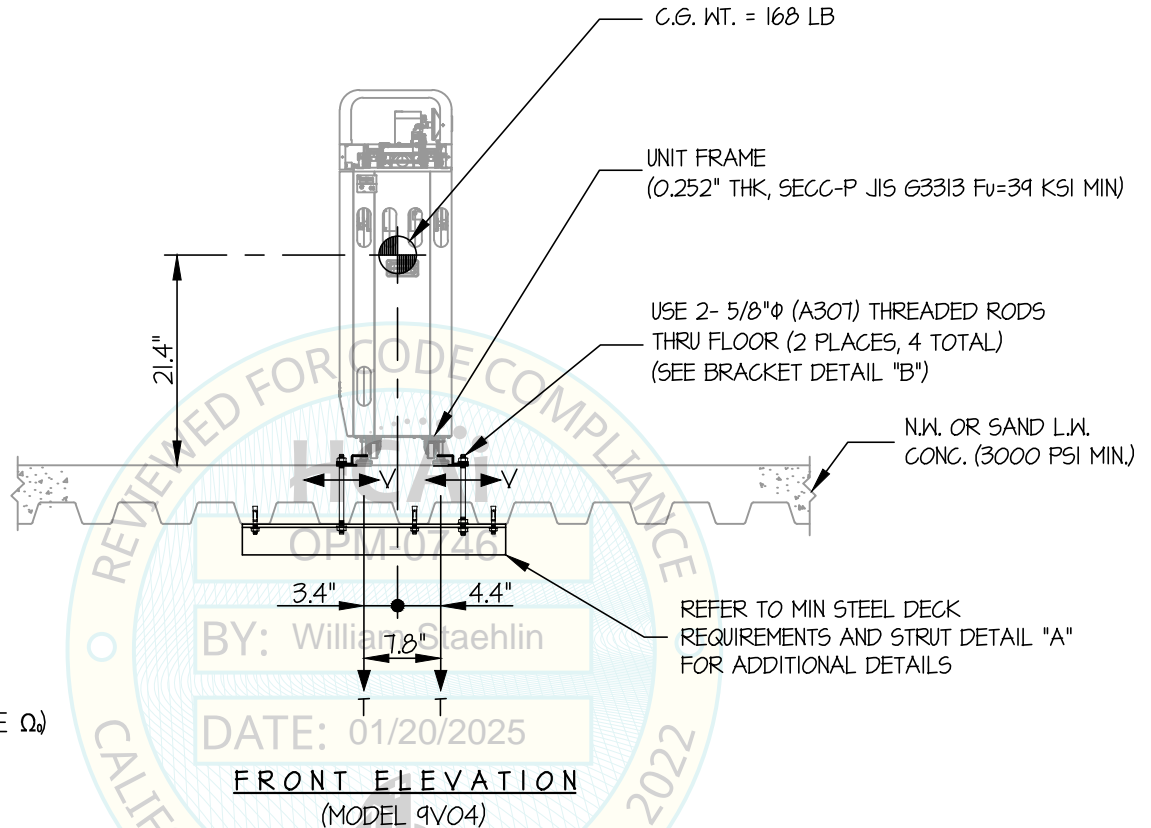

NOTES:

- FORCES ARE DETERMINED PER 2022 CALIFORNIA BUILDING CODE AND ASCE 7-16. STRENGTH DESIGN IS USED. (EXAMPLE: $S_{DS} = 2.30$, $a_p = 1.0$, $I_p = 15$, $R_p = 15$, $\Omega_o = 2.0$, $z/h \leq 1$)

HORIZONTAL FORCE (E_h)	= 2.76	W_p
HORIZONTAL FORCE (E_{mh})	= 5.52	W_p (FOR CONCRETE ANCHORAGE)
VERTICAL FORCE (E_v)	= 0.46	W_p
- THIS PREAPPROVAL ENCOMPASSES WEIGHTS AND VERTICAL C.G. POSITIONS NOT EXCEEDING VALUES SHOWN.
- THIS PREAPPROVAL WAS PREPARED WITHOUT KNOWLEDGE OF ANY SITE CONDITION. COMPATIBILITY FOR USE WITH A SITE SHALL BE EVALUATED BY THE STRUCTURAL ENGINEER OF RECORD OF THE INSTALLATION (SEOR). USE REQUIRES APPROVAL BY THE SEOR.
- STRUCTURAL ENGINEER OF RECORD FOR THE INSTALLATION SHALL VERIFY ALL CONDITIONS, EVALUATE INTERACTION WITH ADJACENT EQUIPMENT AND ANCHORS, AND PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN IN COMBINATION WITH ALL OTHER LOADS THAT MAY BE PRESENT.
- SEE GENERAL NOTES: SHEETS 1 AND 2



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET




17

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

LINK MODULE 3

CONCRETE SLAB ON METAL DECK

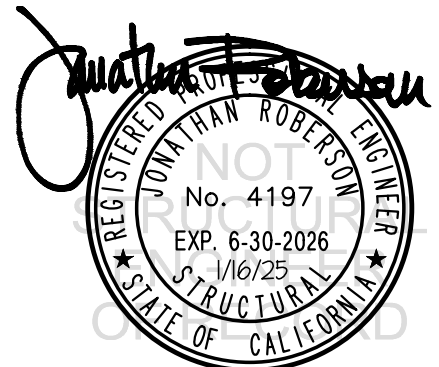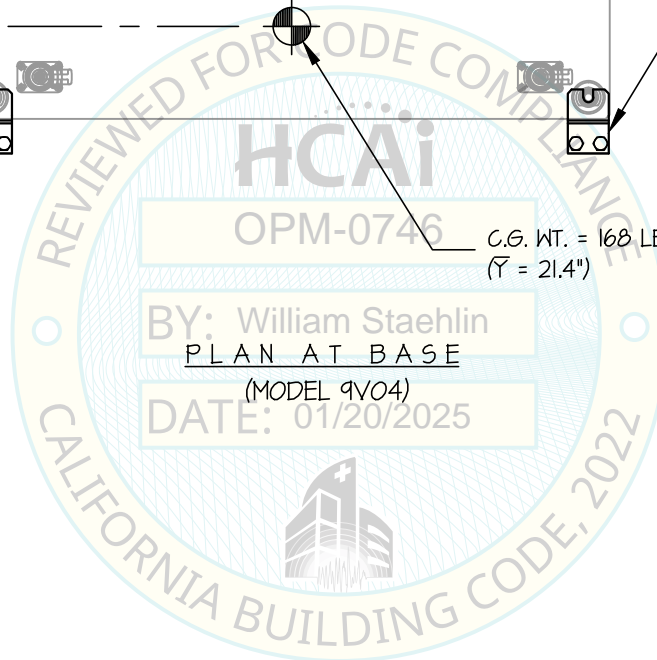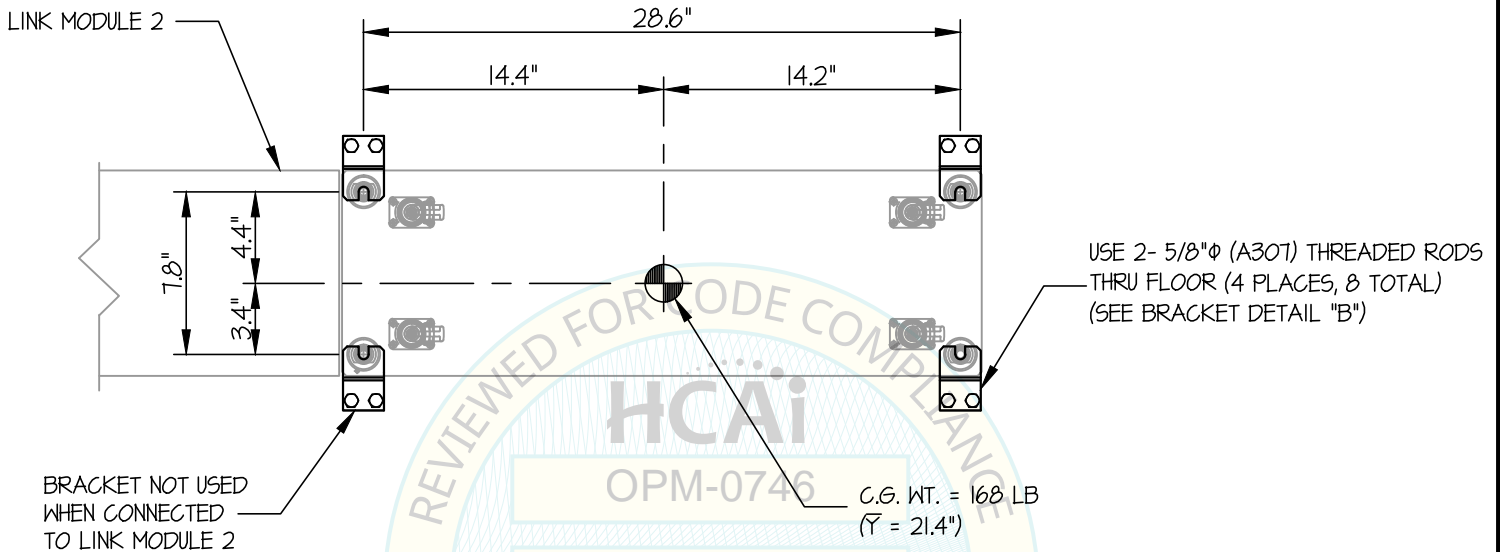

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25

SHEET


18

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS


CONCRETE SLAB ON METAL DECK

LINK MODULE 3
(WHEN REQUIRED)
(MECHANICALLY CONNECTED AT TRACK
TO LINK MODULE 2 W/ (2) M3 (CL 5.8) CAP SCREWS,
CONNECTOR PLATE AND TAPPED BACKING PLATE)
(2 PLACES)

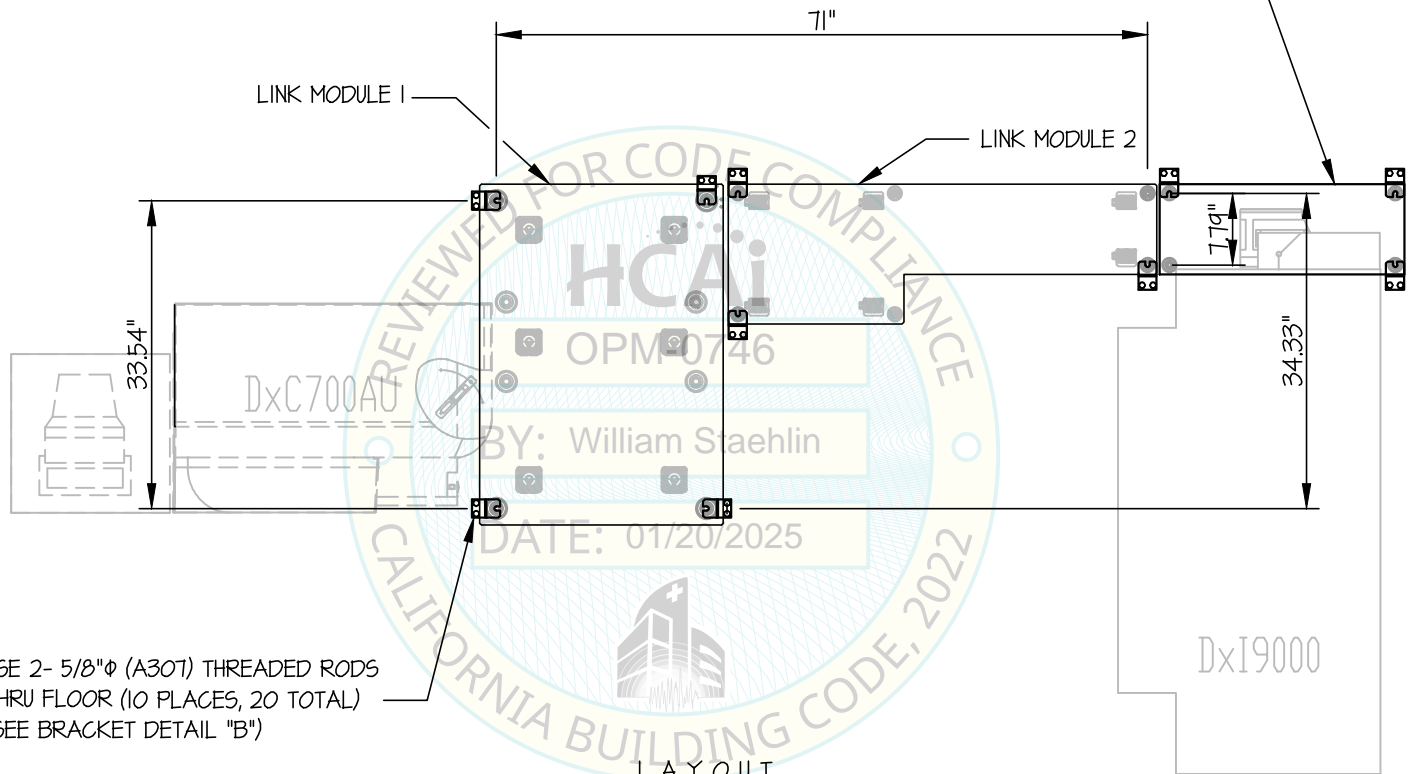

USE 2- 5/8"φ (A307) THREADED RODS
THRU FLOOR (10 PLACES, 20 TOTAL)
(SEE BRACKET DETAIL "B")

LAYOUT
(9720+9722+9V04)

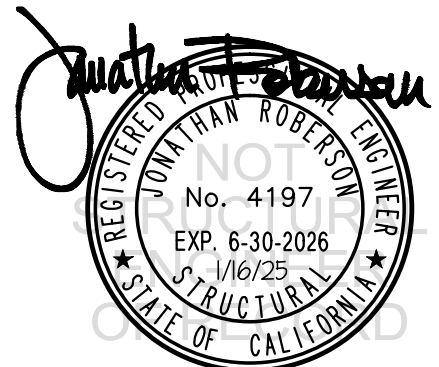

BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25


SHEET

19

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

CONCRETE DETAIL

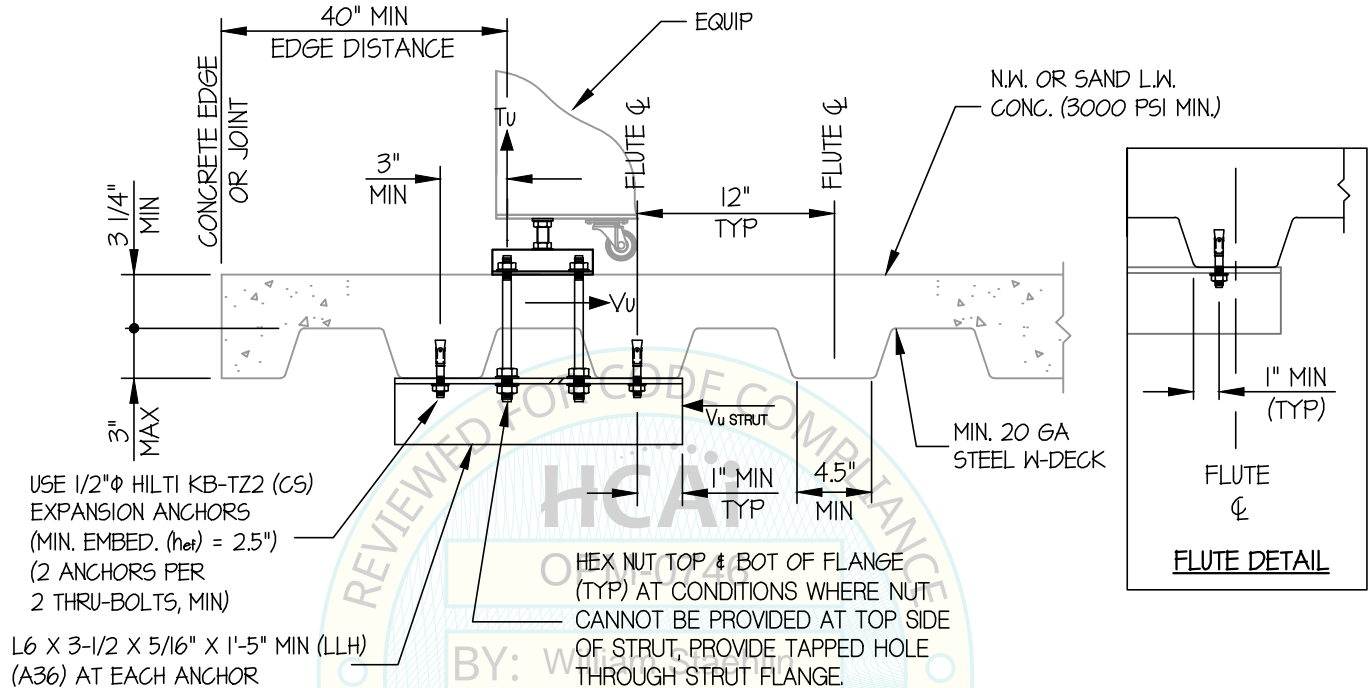

MIN STEEL DECK REQUIREMENTS AND STRUT DETAIL (A)



BECKMAN COULTER

POWERLINK

DES. J. ROBERSON

JOB NO. 11-2412

DATE 1/16/25


SHEET

20

OF 20 SHEETS

SEISMIC SUPPORTS & ATTACHMENTS

BRACKET DETAIL

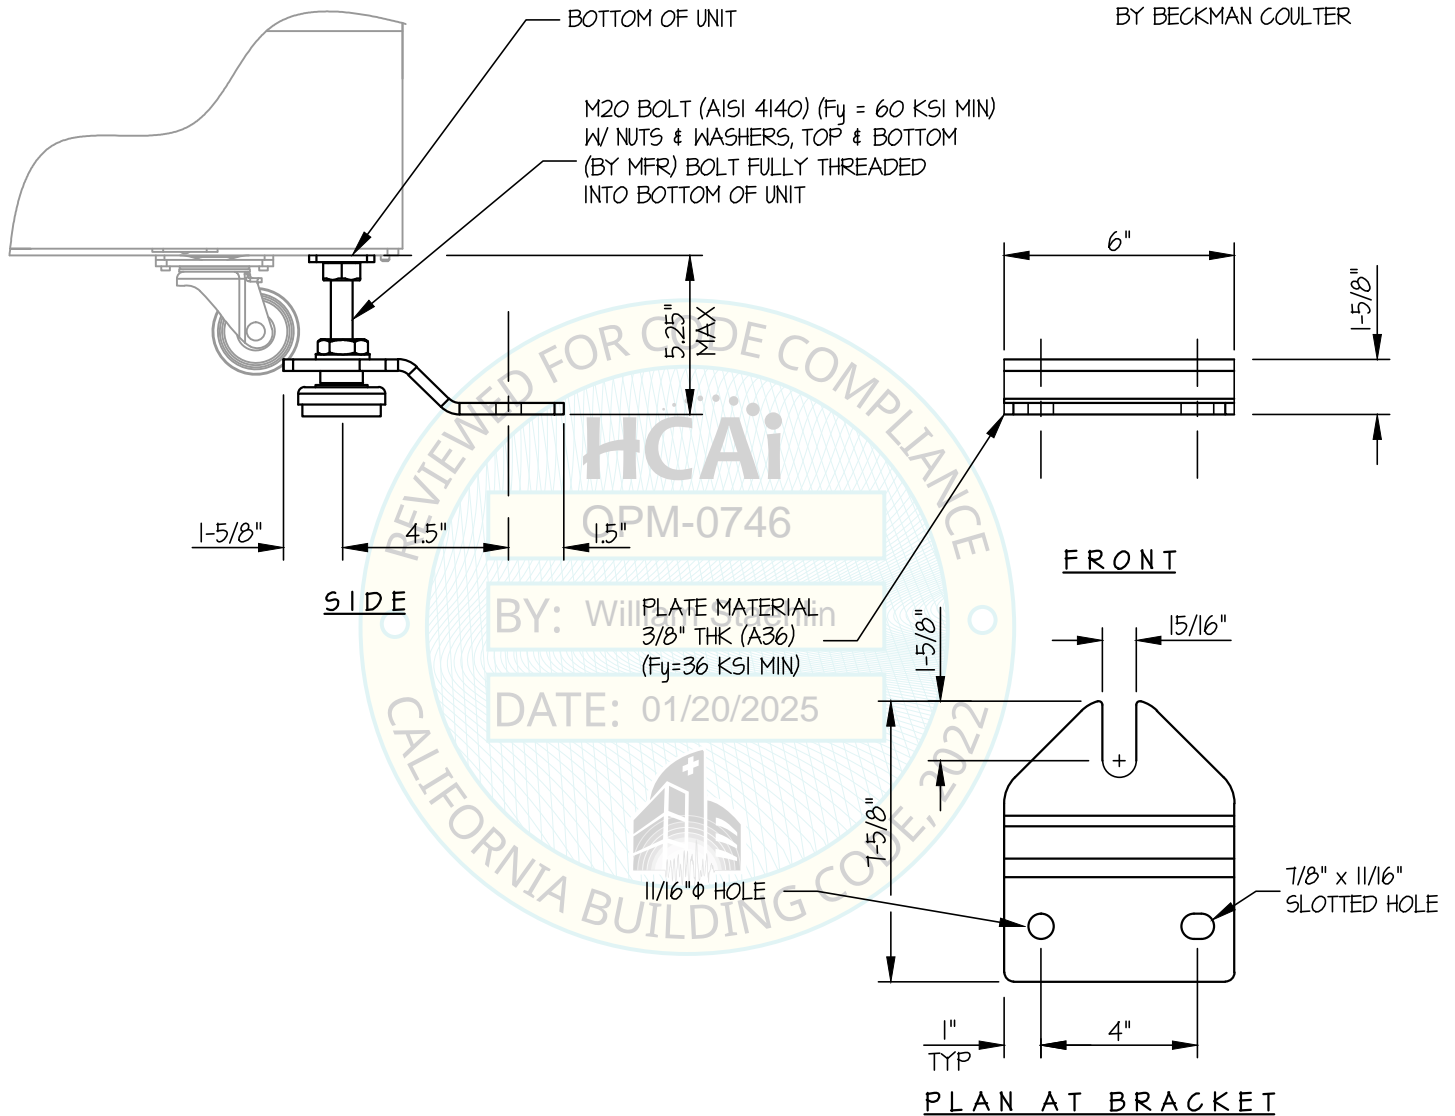NOTE: BRACKET TO BE PROVIDED
BY BECKMAN COULTER

BRACKET DETAIL (B)

