



OFFICE OF STATEWIDE HEALTH PLANNING AND DEVELOPMENT  
FACILITIES DEVELOPMENT DIVISION

APPLICATION FOR OSHPD SPECIAL SEISMIC  
CERTIFICATION PREAPPROVAL (OSP)

OFFICE USE ONLY

APPLICATION #: OSP – 0380 – 10

OSHPD Special Seismic Certification Preapproval (OSP)

Type: ☐ New ☒ Renewal

Manufacturer Information

Manufacturer: Powerex, Inc.

Manufacturer's Technical Representative: Joe Abt, Director of Engineering

Mailing Address: 150 Production Drive, Harrison, OH 45030

Telephone: (513) 367-3273 Email: jabt@powerexinc.com

Product Information

Product Name: Medical Air and Laboratory Air Units, and Medical Gas Automatic Changeover Manifolds

Product Type: Medical gas systems

Product Model Number: See attachment

(List all unique product identification numbers and/or part numbers) OSP-0380-10

General Description: Medical air and laboratory air units contain pumps, a receiver tank, controller and dryers.

Medical gas automatic changeover manifolds are contained in wall mounted enclosures. Seismic enhancements made to the test units and required to address the anomalies observed during the tests shall be incorporated into the production units.

Mounting Description: Medical air and laboratory air units are rigidly base mounted or mounted using neoprene pads.

Medical gas automatic changeover manifolds are rigidly wall mounted.

Applicant Information

Applicant Company Name: The VMC Group

Contact Person: John Giuliano

Mailing Address: 113 Main Street, Bloomingdale, NJ 07403


Telephone: (973) 838-1780 Email: john.giuliano@thvmcgroup.com

I hereby agree to reimburse the Office of Statewide Health Planning and Development review fees in accordance with the California Administrative Code, 2016.

Signature of Applicant:  Date: 1/30/19

Title: President Company Name: The VMC Group

"Access to Safe, Quality Healthcare Environments that Meet California's Diverse and Dynamic Needs"





**OFFICE OF STATEWIDE HEALTH PLANNING AND DEVELOPMENT  
FACILITIES DEVELOPMENT DIVISION**

**California Licensed Structural Engineer Responsible for the Engineering and Test Report(s)**

Company Name: The VMC Group

Name: Kenneth Tarlow California License Number: SE-2851

Mailing Address: 113 Main Street, Bloomingdale, NJ 07403

Telephone: (973) 838-1780 Email: Ken.tarlow@thevmcgroup.com

**Supports and Attachments Preapproval**

☐ Supports and attachments are preapproved under OPM-  
(Separate application for OSHPD Preapproval of Manufacturer's Certification (OPM) of Supports and attachments is required)

☒ Supports and attachments are not preapproved

**Certification Method**

☒ Testing in accordance with: ☒ ICC-ES AC156

☐ Other (Please Specify): \_\_\_\_\_

**Testing Laboratory**

Company Name: Dynamic Certification Laboratories


Contact Name: Josh Sailer, Laboratory Manager

Mailing Address: 1315 Greg Street, Suite 109, Sparks, NV 89431

Telephone: (775) 358-5085 Email: josh@shaketest.com

"Access to Safe, Quality Healthcare Environments that Meet California's Diverse and Dynamic Needs"

STATE OF CALIFORNIA – HEALTH AND HUMAN SERVICES AGENCY  
OSH-FD-759 (REV 12/16/15)



**OSHPD**

Page 2 of 3



# OFFICE OF STATEWIDE HEALTH PLANNING AND DEVELOPMENT FACILITIES DEVELOPMENT DIVISION

## Seismic Parameters

Design in accordance with ASCE 7-10 Chapter 13: ☒ Yes ☐ No

Design Basis of Equipment or Components ( $F_p/W_p$ ) = See attachment

$S_{DS}$  (Design spectral response acceleration at short period, g) = See attachment

$a_p$  (In-structure equipment or component amplification factor) = 2.5

2.5 (systems isolated with neoprene);  
2.0 (internally isolated systems – rigid base mount);  
6.0 (medical gas manifolds)

$R_p$  (Equipment or component response modification factor) = 2.0

$\Omega_0$  (System overstrength factor) = 2.0

$I_p$  (Importance factor) = 1.5

$z/h$  (Height factor ratio) = 1.0

Equipment or Component Natural Frequencies (Hz) = See attachment

Overall dimensions and weight (or range thereof) = See attachment

Equipment or Components @ grade designed in accordance with ASCE 7-10 Chapter 15: ☐ Yes ☒ No

Design Basis of Equipment or Components ( $V/W$ ) = See attachment

$S_{DS}$  (Design spectral response acceleration at short period, g) = See attachment

$S_{D1}$  (Design spectral response acceleration at 1 second period, g) = See attachment

$R$  (Response modification coefficient) = See attachment

$\Omega_0$  (System overstrength factor) = See attachment

$C_d$  (Deflection amplification factor) = See attachment

$I_p$  (Importance factor) = 1.5

Height to Center of Gravity above base = See attachment

Equipment or Component Natural Frequencies (Hz) = See attachment

Overall dimensions and weight (or range thereof) = See attachment

Tank(s) designed in accordance with ASME BPVC, 2015: ☒ Yes ☐ No

## List of Attachments Supporting Special Seismic Certification

- ☒ Test Report(s) ☒ Drawings ☐ Calculations ☐ Manufacturer's Catalog  
☐ Other(s) (Please Specify): \_\_\_\_\_


## OSHPD Approval (For Office Use Only) – Approval Expires on December 31, 2022

Signature: Ali Sumer Date: September 20, 2019

Print Name: Ali Sumer Title: DSE

Special Seismic Certification Valid Up to :  $S_{DS}$  (g) = See above  $z/h$  = See above

Condition of Approval (if applicable): \_\_\_\_\_



**Table 1 - Certified Components - Stacked Units, Medical and Laboratory Scroll - Flexible Base Mount  
(Systems containing 2, 3 and 5 HP Pumps)**

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Systems Containing 2, 3, and 5 HP Pumps														
Medical model number	Laboratory model number <sup>1</sup>	Hp per set	Vertical receiver gallons	Total number of pumps	Vertically stacked pumps or layers	Horizontally arrayed pumps	Maximum dimensions (in) <sup>2</sup>			Max. operating weight (lb) <sup>2</sup>	Mounting <sup>3</sup>	Sds (g), z/h=1	Fp/Wp	Unit
							Length	Width	Height					
Duplex														
MSD0203	LSD0203	2	80	2	2	1	50	31	78	1,040	Flexible base (neoprene) w/ internal isolation	2.00	3.60	UUT1
N/A	LSD0203 (tested with alternate dryer)	2	80	2	2	1	74	32	62	1,090		2.00	3.60	UUT2
MSD0303	LSD0303	3	80	2	2	1	50	31	78	1,100		2.00	3.60	Interpolated
MSD0503	LSD0503	5	80	2	2	1	50	31	78	1,200		2.00	3.60	Interpolated
MSD1004	LSD1004	10	120	4	4	1	78	32	77	1,800		2.00	3.60	Interpolated
MSD1005	N/A	10	200	4	4	1	83	32	84	1,900		2.00	3.60	Interpolated
MSD1506	N/A	15	240	6	2	3	84	66	96	2,820		2.00	3.60	UUT4a/4b
Triplex														
MST0503	N/A	5	80	3	3	1	78	32	70	1,650	Flexible base (neoprene) w/ internal isolation	2.00	3.60	Interpolated
N/A	LST0504	5	120	3	3	1	83	32	77	1,790		2.00	3.60	Interpolated
MST1005	LST1005	10	200	6	2	3	90	66	84	2,800		2.00	3.60	Interpolated
MST1505	N/A	15	200	9	3	3	90	66	84	3,900		2.00	3.60	Interpolated
Quadruplex														
MSQ0504	LSQ0504	5	120	4	4	1	77	32	77	1,870	Flexible base (neoprene) w/ internal isolation	2.00	3.60	UUT3
MSQ1005	LSQ1005	10	200	8	2	4	108	66	84	3,400		2.00	3.60	Interpolated
MSQ1006	N/A	10	240	8	2	4	108	66	96	3,530		2.00	3.60	Interpolated
MSQ1505	N/A	15	200	12	3	4	108	66	84	4,200		2.00	3.60	Interpolated
MSQ1506	N/A	15	240	12	3	4	108	66	96	4,260		2.00	3.60	UUT5b/UUT7
Pentaplex														
MSP0504	N/A	5	120	5	1, 2	2	84	66	77	2,475	Flexible base (neoprene) w/ internal isolation	2.00	3.60	Extrapolated <sup>4</sup>
MSP0505	N/A	5	200	5	1, 2	2	84	66	84	2,600		2.00	3.60	Extrapolated <sup>4</sup>
MSP1505	N/A	15	200	15	2, 3	3	90	148	84	5,100		2.00	3.60	Extrapolated <sup>4</sup>
MSP1506	N/A	15	240	15	2, 3	3	90	148	96	5,300		2.00	3.60	Extrapolated <sup>4</sup>
Hexaplex														
MSH0504	N/A	5	120	6	2	3	90	66	77	2,835	Flexible base (neoprene) w/ internal isolation	2.00	3.60	Extrapolated <sup>4</sup>
MSH0505	N/A	5	200	6	2	3	90	66	84	2,975		2.00	3.60	Extrapolated <sup>4</sup>
MSH1006	N/A	10	240	12	3	4	108	73	96	4,250		2.00	3.60	Extrapolated <sup>4</sup>
MSH1506	N/A	15	240	18	3, 3	3	94	150	96	6,020		2.00	3.60	Extrapolated <sup>4</sup>
Seven to Twelve Pump Systems														
MSO0504	N/A	5	120	7	2	4 lower, 3 upper	103	66	82	2,900	Flexible base (neoprene) w/ internal isolation	2.00	3.60	Extrapolated <sup>4</sup>
MSO0505	N/A	5	200	7	2	4 lower, 3 upper	103	66	84	3,190		2.00	3.60	Extrapolated <sup>4</sup>
MSO0505	N/A	5	200	8	2	4	103	66	84	3,350		2.00	3.60	Extrapolated <sup>4</sup>
MSN0505	N/A	5	200	9	3	3	94	66	84	3,900		2.00	3.60	Extrapolated <sup>4</sup>
MSJ0505	N/A	5	200	10	3	4 lower, 4 mid, 2 upper	104	66	84	3,700		2.00	3.60	Extrapolated <sup>4</sup>
MSJ0506	N/A	5	240	10	3	4 lower, 4 mid, 2 upper	104	66	96	3,900		2.00	3.60	Extrapolated <sup>4</sup>
MSK0505	N/A	5	200	11	3	4 lower, 4 mid, 3 upper	104	66	84	3,900		2.00	3.60	Extrapolated <sup>4</sup>
MSK0506	N/A	5	240	11	3	4 lower, 4 mid, 3 upper	104	66	96	4,175		2.00	3.60	Extrapolated <sup>4</sup>
MSL0505	N/A	5	200	12	3	4	104	66	84	4,100		2.00	3.60	Extrapolated <sup>4</sup>
MSL0506	N/A	5	240	12	3	4	104	66	96	4,360		2.00	3.60	Extrapolated <sup>4</sup>

**Notes:**

1. Lab scroll units differ from medical scroll units by software change only.
2. Maximum dimensions and weights relate to options and receiver tank size.
3. Pump skids feature internal isolation. Skids with only dryers and tanks do not.
4. Extrapolated unit justification matrix is provided following this table.



**Table 2 - Certified Components - Stacked Units, Medical and Laboratory Scroll - Rigid Base Mount  
(Systems Containing 2, 3 and 5 HP Pumps)**

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Systems Containing 2, 3, and 5 HP Pumps															
Medical model number	Laboratory model number <sup>1</sup>	Hp per set	Vertical receiver gallons	Total number of pumps	Vertically stacked pumps or layers	Horizontally arrayed pumps	# independently mounted & plumbed assemblies	Maximum dimensions (in) <sup>2</sup>			Max. operating weight (lb) <sup>2</sup>	Mounting <sup>3</sup>	Sds (g), z/h=1	Fp/Wp	Unit
								Length	Width	Height					
Duplex															
MSD02A3	LSD02A3	2	80	2	2	1	1	50	34	74	1,090	Rigid base w/ internal isolation	2.00	4.50	UUT 32
MSD03A3	LSD03A3	3	80	2	2	1	1	50	34	74	1,120		2.00	4.50	Interpolated
MSD05A3	LSD05A3	5	80	2	2	1	1	50	34	74	1,300		2.00	4.50	Interpolated
MSD10A4	LSD10A4	10	120	4	4	1	2	51	73	75	2,120		2.00	4.50	Interpolated
MSD10A5	LSD10A5	10	200	4	4	1	2	51	73	85	2,360		2.00	4.50	Interpolated
MSD10A6	LSD10A6	10	240	4	4	1	2	51	73	94	2,470		2.00	4.50	Interpolated
MSD15A5	LSD15A5	15	200	6	2	3	2	60	73	86	3,030		2.00	4.50	Interpolated
MSD15A6	LSD15A6	15	240	6	2	3	2	60	73	94	3,090	2.00	4.50	Interpolated	
Triplex															
MST03A3	LST03A3	3	80	3	3	1	2	51	73	74	1390	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MST05A3	LST05A3	5	80	3	3	1	2	51	73	74	1720		2.00	4.50	Interpolated
MST05A4	LST05A4	5	120	3	3	1	2	51	73	75	1,936		2.00	4.50	Interpolated
MST10A4	LST10A4	10	120	6	3	2	2	60	73	75	2,995		2.00	4.50	Interpolated
MST10A5	LST10A5	10	200	6	3	2	2	60	73	86	3230		2.00	4.50	Interpolated
MST10A6	LST10A6	10	240	6	3	2	2	60	73	94	3320		2.00	4.50	Interpolated
MST15A4	LST15A4	15	120	9	3	3	2	73	73	75	3930		2.00	4.50	Interpolated
MST15A5	LST15A5	15	200	9	3	3	2	73	73	86	4201		2.00	4.50	Interpolated
MST15A6	LST15A6	15	240	9	3	3	2	73	73	94	4260	2.00	4.50	Interpolated	
Quadruplex															
MSQ05A4	LSQ05A4	5	120	4	4	1	1	51	73	75	2,180	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSQ10A5	LSQ10A5	10	200	8	2	4	2	60	73	86	3,790		2.00	4.50	Interpolated
MSQ10A6	LSQ10A6	10	240	8	2	4	2	60	73	94	3,840		2.00	4.50	Interpolated
MSQ15A5	LSQ15A5	15	200	12	3	4	2	73	73	86	5,620		2.00	4.50	Interpolated
MSQ15A6	LSQ15A6	15	240	12	3	4	2	73	73	94	5,680		2.00	4.50	Interpolated
Pentaplex															
MSP15A5	LSP15A5	15	200	15	3,4,4,4	4	2	85	73	86	6,080	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSP15A6	LSP15A6	15	240	15	3,4,4,4	4	2	86	73	91	6,140		2.00	4.50	UUT 33i,ii
Hexaplex															
MSH05A4	LSH05A4	5	120	6	2	3	2	60	75	75	2,990	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSH05A5	LSH05A5	5	200	6	2	3	2	60	75	86	3,230		2.00	4.50	Interpolated
MSH10A6	LSH10A6	10	240	12	3	4	2	73	73	94	5,680		2.00	4.50	Interpolated
MSH15A5	LSH15A5	15	200	18	3	6	3	85	113	86	7,750		2.00	4.50	Extrapolated <sup>4</sup>
MSH15A6	LSH15A6	15	240	18	3	6	3	85	113	94	7,810		2.00	4.50	Extrapolated <sup>4</sup>
Nine-plex															
MSN05A5	LSN05A5	5	200	9	3	3	2	73	73	86	4,680	Rigid base w/ internal isolation	2.00	4.50	Interpolated

**Notes:**


1. Lab scroll units differ from medical scroll units by software change only.
2. Maximum dimensions and weights relate to options and receiver tank size.
3. Pump skids feature internal isolation. Skids with only dryers and tanks do not.
4. Extrapolated unit justification matrix is provided following this table.

**Table 3 - Justification Matrix for Extrapolation - Stacked Units, Medical and Laboratory Scroll  
(Systems containing 2, 3 and 5 HP Pumps)**

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Systems Containing 2, 3 and 5 HP Pumps			
Extrapolated unit (medical)	Extrapolated unit (laboratory)	Units used for extrapolation	Difference from units used for extrapolation
MSP0504	N/A	UUT4 (MSD1504)	One fewer pump
MSP0505	N/A	UUT4 (MSD1504)	One fewer pump, larger 200 gal receiver (240 gal receiver tested in UUT5b/UUT7)
MSP1505	N/A	Interpolated unit MST1505	Has an additional pump skid like that tested in UUT4, includes 24" spacing between each of the skids
MSP1506	N/A	Interpolated unit MST1505	Has an additional pump skid like that tested in UUT4 and includes 24" spacing between each of the skids.
MSH0504	N/A	UUT4 (MSD1504)	Has 6 pumps in rack of 3, 3 layers
MSH0505	N/A	UUT4 (MSD1504)	Has 6 pumps in rack of 3, 3 layers, and larger 200 gal receiver (240 gal receiver tested in UUT5b/UUT7)
MSH1006	N/A	UUT5b/UUT7 (MSQ1506)	Includes 6" space between the two system frame modules.
MSH1506	N/A	Interpolated unit MST1505	Has additional pump skid and includes 24" spacing between each of the skids, with 240 gal receiver like that tested in UUT5
MSS0504	N/A	UUT5b/UUT7 (MSQ1506)	One less row of pumps, with smaller receiver tank (one pump less than interpolated MSQ1005)
MSS0505	N/A	UUT5b/UUT7 (MSQ1506)	One less row of pumps, with smaller receiver tank (one pump less than interpolated MSQ1005)
MSO0505	N/A	UUT5b/UUT7 (MSQ1506)	One less row of pumps, with smaller receiver tank
MSN0505	N/A	UUT5b/UUT7 (MSQ1506)	One less column of pumps, with smaller receiver tank
MSJ0505	N/A	UUT5b/UUT7 (MSQ1506)	Two fewer pumps in the top row, with smaller receiver tank
MSJ0506	N/A	UUT5b/UUT7 (MSQ1506)	Two fewer pumps in the top row
MSK0505	N/A	UUT5b/UUT7 (MSQ1506)	One fewer pump in the top row, with smaller receiver tank
MSK0506	N/A	UUT5b/UUT7 (MSQ1506)	One fewer pump in the top row
MSL0505	N/A	UUT5b/UUT7 (MSQ1506)	Smaller receiver tank
MSL0506	N/A	UUT5b/UUT7 (MSQ1506)	Software change only
MSH15A5	N/A	UUT32/UUT33 (MST15A5)	Same pump rack duplicated, tank, dryer, and controller from UUT4
MSH15A6	N/A	UUT32/UUT33 (MST15A6)	Same pump rack duplicated, tank, dryer, and controller from UUT4

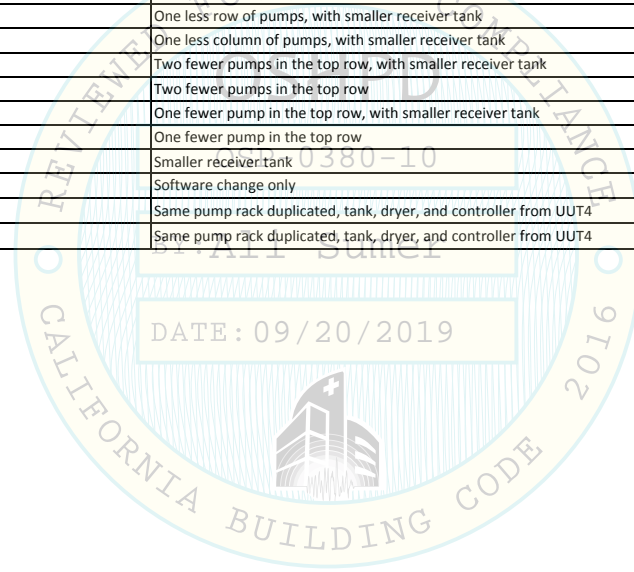

**Table 4 - Certified Components - Stacked Units, Medical and Laboratory Scroll  
(Systems Containing 7.5 and 10 HP Pumps, Rigid Base Mount)**

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Systems Containing 7.5 and 10 HP Pumps - Rigid Base Mount														
Medical air Model number	Laboratory Air Model number <sup>1</sup>	Hp per set	Vertical receiver gallons	Total number of pumps	Vertically stacked pumps or layers	Horizontally arrayed pumps	Max. dimensions (in) <sup>2</sup>			Max. operating Weight (lb) <sup>2</sup>	Mounting <sup>3</sup>	Sds(g), z/h=1	Fp/Wp	Unit
							Length	Width	Height					
Systems with 80 to 240 Gallon Tanks														
Duplex														
MSD0753	LSD0753	7.5	80	2	2	1	66	61	68	2,205	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>4</sup>
MSD0754	LSD0754	7.5	120	2	2	1	66	61	78	2,260		2.00	4.50	Extrapolated <sup>4</sup>
MSD10B4	LSD10B4	10	120	2	2	1	66	61	78	2,310		2.00	4.50	Extrapolated <sup>4</sup>
MSD15B4	LSD15B4	15	120	4	4	1	66	61	78	2,390		2.00	4.50	UUT10a/10b
MSD20B4	LSD20B4	20	120	4	4	1	66	61	78	2,500		2.00	4.50	Interpolated
Triplex														
MST0755	LST0755	7.5	200	3	3	1	66	61	81	2,400	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MST10B5	LST10B5	10	200	3	3	1	66	61	81	2,550		2.00	4.50	Interpolated
MST15B5	LST15B5	15	200	6	3	2	90	79	81	4,200		2.00	4.50	Interpolated
MST15B6	LST15B6	15	240	6	3	2	90	79	93	4,300		2.00	4.50	Interpolated
MST20B5	LST20B5	20	200	6	3	2	90	79	81	4,450		2.00	4.50	Interpolated
MST20B6	LST20B6	20	240	6	3	2	90	79	93	4,550		2.00	4.50	Interpolated
Quadruplex														
MSQ0755	LSQ0755	7.5	200	4	4	1	61	66	81	2,650	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSQ10B5	LSQ10B5	10	200	4	4	1	61	66	81	2,750		2.00	4.50	Interpolated
MSQ15B5	LSQ15B5	15	200	8	4	2	90	79	81	4,450		2.00	4.50	Interpolated
MSQ15B6	LSQ15B6	15	240	8	4	2	90	79	93	4,550		2.00	4.50	Interpolated
MSQ20B5	LSQ20B5	20	200	8	4	2	90	79	81	4,700		2.00	4.50	Interpolated
MSQ20B6	LSQ20B6	20	240	8	4	2	90	79	93	4,800		2.00	4.50	UUT11ai/bii
Pentaplex														
MSP15B6	LSP15B6	15	240	10	4 max, partial fill	3	138	76	93	7,000	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>4</sup>
MSP20B6	LSP20B6	20	240	10	4 max, partial fill	3	138	76	93	7,200		2.00	4.50	Extrapolated <sup>4</sup>
Systems with 400 or 660 Gallon Tanks (Tank separately mounted and flexibly plumbed)														
Pentaplex														
MSP15B7	LSP15B7	15	400	10	4 max, partial fill	3	158	96	102	7,400	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT12c tank
MSP20B7	LSP20B7	20	400	10	4 max, partial fill	3	158	96	102	7,600		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT12c tank
MSP15B8	LSP15B8	15	660	10	4 max, partial fill	3	163	99	127	8,100		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT15b tank
MSP20B8	LSP20B8	20	660	10	4 max, partial fill	3	163	99	127	8,300		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT15b tank
Hexaplex														
MSH15B7	LSH15B7	15	400	12	4	3	158	96	102	8,600	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT12c tank
MSH20B7	LSH20B7	20	400	12	4	3	158	96	102	9,000		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT12c tank
MSH15B8	LSH15B8	15	660	12	4	3	163	99	127	9,300		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT15b tank
MSH20B8	LSH20B8	20	660	12	4	3	163	99	127	9,700		2.00	4.50	Extrapolated <sup>4</sup> , w/ UUT15b tank
400 and 660 Gallon Tanks														
Tank Model No.	Description					Max. dimensions (in)			Weight (lb)	Mounting	Sds(g), z/h=1	Fp/Wp	Unit	
						Length	Width	Height						
AR063700AV	400 gal					38	47	102	640	Rigid base	2.00	2.40	UUT12c	
AR660000AV	660 gal					42	42	127	1,500		2.00	2.40	UUT15b	

**Notes:**

1. Lab scroll units differ from medical scroll units by software change only.
2. Maximum dimensions and weights are calculated, and take into account options and receiver tank size.
3. Pump skids feature internal isolation. Skids with dryers and tanks do not.
4. Extrapolated unit justification matrix is provided following this table.

**Table 5 - Justification Matrix for Extrapolation - Stacked Units, Medical and Laboratory Scroll  
(Systems Containing 7.5 and 10 HP Pumps)**

<b>Manufacturer:</b> Powerex			
<b>Product Line:</b> Medical Air and Laboratory Air			
Extrapolated unit (medical)	Extrapolated unit (laboratory)	Units used for extrapolation	Difference from units used for extrapolation
MSD0753	LSD0753	UUT10 (MSD15B4)	Two fewer pump-motor assemblies in rack; tank is smaller from UUT 1
MSD0754	LSD0754	UUT10 (MSD15B4)	Two fewer pump-motor assemblies in rack.
MSD10B4	LSD10B4	UUT10 (MSD15B4)	Two fewer pump-motor assemblies in rack, pump-motor assemblies as in UUT11
MSP15B6	LSP15B6	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506)	10 total pumps; one 2 pump stack, as a depopulated variant of UUT10 control deleted, one 8 pump (2 stacks -4 high, using 7.5HP pumps and motors instead of 10HP) as in UUT11; Control depopulated variant of UUT7 (10 of 12 circuits); Tank/dryer skid as in UUT5b with dryers as in UUT6 or UUT9
MSP20B6	LSP20B6	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506)	10 total pumps; One 2 pump stack, as a depopulated variant of UUT10 with 10 HP pumps/motors instead of 7.5 control deleted, one 8 pump (2stack -4 high) as in UUT11; Control depopulated variant of UUT7 (10 of 12 circuits). Tank/dryer skid as in UUT5b with dryers as in UUT6 or UUT9
MSH15B6	LSH15B6	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506)	12 total pumps; one 4 pump stack, as in UUT10; one 8 pump stack (2 stacks -4 high, using 7.5HP pumps and motors instead of 10HP) as in UUT11; Controller tested in UUT7. Tank/dryer skid as in UUT5b with dryers as in UUT6 or UUT9.
MSH20B6	LSH20B6	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506)	12 total pumps; One 4 pump stack, as in UUT10 with 10 HP pumps/motors instead of 7.5 (10HP covered by interpolation to UUT10-11); one 8 pump stack (2 stacks -4 high) as in UUT11; Controller a depopulated variant of UUT7 (10 of 12 circuits). Tank/dryer skid as in UUT5b with dryers as in UUT6 or UUT9
MSP15B7	LSP15B7	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT12c (400gal receiver)	Same as MSP15B6 above, except tank/dryer skid deletes receiver tank, add separately mounted/flexibly plumbed 400gal receiver as in UUT12c
MSP20B7	LSP20B7	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT12c (400gal receiver)	Same as MSP20B6 above, except tank/dryer skid deletes receiver tank, add separately mounted/flexibly plumbed 400gal receiver as in UUT12c
MSP15B8	LSP15B8	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT15b (660gal receiver)	Same as MSP15B6 above, except tank/dryer skid deletes receiver tank, add separately mounted/flexibly plumbed 660gal receiver as in UUT15b
MSP20B8	LSP20B8	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT15b (660gal receiver)	Same as MSP20B6 above, except tank/dryer skid deletes receiver tank, add separately mounted/flexibly plumbed 660gal receiver as in UUT15b
MSH15B7	LSH15B7	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT12c (400gal receiver)	Same as MSH15B6 above, except tank/dryer skid deletes receiver tank; add separately mounted/flexibly plumbed 400gal receiver as in UUT12c
MSH20B7	LSH20B7	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT12c (400gal receiver)	Same as MSH20B6 above, except tank/dryer skid deletes receiver tank; add separately mounted/flexibly plumbed 400gal receiver as in UUT12c
MSH15B8	LSH15B8	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT15b (660gal receiver)	Same as MSH15B6 above, except tank/dryer skid deletes receiver tank; add separately mounted/flexibly plumbed 660gal receiver as in UUT15b
MSH20B8	LSH20B8	UUT10 (MSD15B4), UUT11(MSQ20B6), UUT7(MSQ1506), UUT15b (660gal receiver)	Same as MSH20B6 above, except tank/dryer skid deletes receiver tank; add separately mounted/flexibly plumbed 660gal receiver as in UUT15b

**Table 6 - Certified Subcomponents - Stacked Units, Medical and Laboratory Scroll (Flexible Base Mount)**

Subcomponent [MFR]	Model	Notes	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
<b>Scroll pumps</b> [POWEREX] Note: material is die cast aluminum	SLAE03EB	2 or 3 Hp	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2
	SLAE05E	5 Hp		2.00	3.60	UUT3
	SLAE05EHP	5 Hp		2.00	3.60	Same as UUT3
<b>Vertical tanks</b> [CAMPBELL HAUSFELD, ALSO BRANDED TWIN LAKES] Note: material is welded carbon steel	AR027300ST	80 gal	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2
	AR027400ST	120 gal		2.00	3.60	UUT3
<b>Dew point monitor / probe desiccant</b> [POWEREX] Note: material of probe housing is stainless steel	PDPM1001AJ	N/A	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2, UUT3
	PDMP2001AJ	N/A		2.00	3.60	Extrapolated <sup>1</sup>
<b>Carbon monoxide monitor/ sensor</b> [ENMET] Note: material is FRP housing with circuit board and integrated sensor	03481-005	N/A	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2, UUT3
<b>Controllers</b> [POWEREX] Note: material is painted carbon steel electrical cabinet	BASIC_PSM	NEMA 12 enclosure; No Touchscreen	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1
	HMI_PXMI	NEMA 12 enclosure: Human Machine Interface		2.00	3.60	Interpolated
	PBMI_PXMI	NEMA 12 enclosure: Powerex Building Management Integrator		2.00	3.60	UUT2, UUT3
<b>Motors</b> [WEG] Note: material is carbon steel shell with welded foot Note: All motors are 208-230V / 460V	002180T3E145T	2 Hp	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2
	002180T3ECD145T	2 Hp		2.00	3.60	Interpolated
	003180T3E182T	3 Hp		2.00	3.60	Interpolated
	005180T3E184T	5 Hp		2.00	3.60	UUT3
<b>Tank drain</b> [JORC] Note: material is cast brass body with integrated solenoid valve and DIN connector-mounted solid state timer	2523	Timer Drain	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT3
<b>Tank drain</b> [PARKER-DOMNICK HUNTER / ZANDER] Note: material is die cast body and molded polymer housing	ED3004N	No-Loss Drain	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT2
<b>Aftercooler</b> [THERMAL TRANSFER] Note: material is copper header tanks, copper cross tubes and copper fins	DH062	N/A	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2, UUT3
<b>Intake filter elements</b> [SOLBERG] Note: material is powder-coated stamped carbon steel	CSL-843	MSD0203, MSD0303, MSD0503, MST0503, MSP1505	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1
	CSL-849	MSQ0504, MSH0504, MSD1504, SDT1005, MSP1505		2.00	3.60	UUT2
	CSL-851	MSN0504, MST1505, MSQ1005, MSQ1505, MSL0505, MSO0505		2.00	3.60	UUT7
<b>Check valve</b> [POWEREX] Note: material is anodized die cast aluminum	IP087700AV	Check Valve	Flexible base (neoprene) w/ internal Isolation	2.00	3.60	UUT1, UUT2, UUT3
<b>Vertical tanks</b> [CAMPBELL HAUSFELD, ALSO BRANDED TWIN LAKES] Note: material is welded carbon steel	AR051201AJ	200 gal	Flexible base (neoprene)	2.00	3.60	Extrapolated
	AR051301AJ	240 gal		2.00	3.60	UUT4b, UUT5b
<b>Vertical tanks</b> [Morganton] Note: material is welded carbon steel	VES07285	80 gal	Flexible base (neoprene)	2.00	3.60	UUT 30b, UUT 31b
	VES04865	120 gal				Interpolated
	VES04767	120 gal				UUT 31b
	VES07303	200 gal				Interpolated
	VES07072	240 gal				UUT 30b

1. Extrapolated dew point monitor is the same as tested in UUT1-3 (software change only).

**Table 6 - Certified Subcomponents (Continued) - Stacked Units, Medical and Laboratory Scroll  
(Flexible Base Mount)**

Subcomponent [MFR]	Model <sup>1</sup>	Dimensions (in)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
		Length	Width	Height					
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame	PMD10	17	28	53	200	Flexible base (neoprene), w/ or w/out internal isolation	2.00	3.60	Extrapolated
	PMD17	17	28	53	200		2.00	3.60	Extrapolated
	PMD30	17	28	64	330		2.00	3.60	UUT3
	PMD35	17	28	64	330		2.00	3.60	Interpolated
	PMD45	17	28	72	360		2.00	3.60	Interpolated
	PMD55	17	28	72	360		2.00	3.60	Interpolated
	PMD60	35	28	67	660		2.00	3.60	Interpolated
	PMD71	35	28	67	660		2.00	3.60	Interpolated
	PMD90	35	28	76	720		2.00	3.60	Interpolated
	PMD110	35	28	76	720		2.00	3.60	Interpolated
	PMD111	35	28	76	720		2.00	3.60	UUT4b
	PMD07T	18	28	37	185		2.00	3.60	UUT1
	PMD10T	18	28	37	185		2.00	3.60	Extrapolated <sup>2</sup>
	PMD17T	18	28	37	185		2.00	3.60	Extrapolated <sup>2</sup>
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame	PLD10	17	28	53	200	Flexible base (neoprene), w/ or w/out internal isolation	2.00	3.60	Extrapolated
	PLD17	17	28	53	200		2.00	3.60	Extrapolated
	PLD30	17	28	64	330		2.00	3.60	UUT3
	PLD35	17	28	64	330		2.00	3.60	Interpolated
	PLD45	17	28	72	360		2.00	3.60	Interpolated
	PLD55	17	28	72	360		2.00	3.60	Interpolated
	PLD60	35	28	67	660		2.00	3.60	Interpolated
	PLD71	35	28	67	660		2.00	3.60	Interpolated
	PLD90	35	28	76	720		2.00	3.60	Interpolated
	PLD111	35	28	76	720		2.00	3.60	UUT4b
	PLD07T	18	28	37	185		2.00	3.60	UUT1
	PLD10T	18	28	37	185		2.00	3.60	Extrapolated <sup>2</sup>
	PLD17T	18	28	37	185		2.00	3.60	Extrapolated <sup>2</sup>
<b>Desiccant dryers</b> [PARKER-DOMNICK, alternately branded HUNTER/ZANDER]  Note: material is aluminum extruded towers; powder coated welded carbon steel mounting frame	DME050RX	22	9	56	176	Flexible base (neoprene), w/ or w/out internal isolation	2.00	3.60	UUT5b
	DME060RX	22	9	63	198		2.00	3.60	Interpolated
	DME080RX	22	9	73	229		2.00	3.60	UUT6
	DME015	12	11	33	81		2.00	3.60	UUT6
	DME025	12	11	53	103		2.00	3.60	Interpolated
	DME030	12	11	59	114		2.00	3.60	Interpolated
	DME050	22	9	56	176		2.00	3.60	Interpolated
	DME060	22	9	63	198		2.00	3.60	UUT6
	KMT3	8	12	32	37		2.00	3.60	UUT2
	KMT4	8	12	54	54		2.00	3.60	UUT6
<b>Desiccant dryers</b> [NANO PSI] Note: material is aluminum extruded towers; powder coated carbon steel mounting frame	NDL110	17	13	48	172	Flexible base (neoprene)	2.00	3.60	UUT9
	NDL120	17	13	52	209		2.00	3.60	Interpolated
	NDL130	17	13	56	262		2.00	3.60	Interpolated
	NDL2110	25	12	47	366		2.00	3.60	UUT9

Notes:

1. Dryers with PLD designation are structurally identical to PMD models in chart above.

2. The PMD10T/PLD10T and PMD17T/PLD17T are identical to the PMD07T/PLD07T.



**Table 7 - Certified Subcomponents - Stacked Units, Medical and Laboratory Scroll  
(Rigid Base Mount)**

Subcomponent [MFR]	Model	Notes	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
<b>Scroll pumps</b> [POWEREX] Note: material is die cast aluminum	SLAE075	7.5 Hp	Rigid base w/ internal Isolation	2.00	4.50	UUT10a
	SLAE10	10 Hp		2.00	4.50	UUT11aii
<b>Controllers</b> [POWEREX] Note: material is painted carbon steel electrical cabinet	BASIC_PSM	NEMA 12 enclosure; No Touchscreen	Rigid base w/ internal Isolation	2.00	4.50	UUT10a
	HMI_PXMI	NEMA 12 enclosure: Human Machine Interface: Touchscreen		2.00	4.50	Interpolated
	PBMI_PXMI	NEMA 12 enclosure: Powerex Building Management Integrator: HMI panel with additional communications card		2.00	4.50	UUT11aii
<b>Motors for medical and lab skid mount</b> [WEG] Note: material is carbon steel shell with welded foot Note: All motors are 208-230V / 460V	007360T2E184T	7.5 Hp	Rigid base w/ internal Isolation	2.00	4.50	UUT10a
	010360T3E213T	10 Hp		2.00	4.50	UUT11aii
<b>Aftercooler</b> [THERMAL TRANSFER] Note: material is copper header tanks, copper cross tubes and copper fins	BGA35	N/A	Rigid base w/ internal Isolation	2.00	4.50	UUT 32,33ii
	DH106	N/A		2.00	4.50	UUT10a, UUT11aii
<b>Intake filter elements</b> [SOLBERG] Note: material is powder-coated stamped carbon steel	CSL-824	Multiple filters used per unit, up to one per pump	Rigid base w/ internal Isolation	2.00	4.50	UUT 32, 33ii
	CSL-849	Multiple filters used per unit, up to one per pump		2.00	4.50	UUT10a, UUT11aii
<b>Check valve</b> [CONTROL DEVICES, INC.] Note: material is cast brass	CB50	Check Valve	Rigid base w/ internal Isolation	2.00	4.50	UUT10a, UUT11aii
<b>Vertical tanks</b> [CAMPBELL HAUSFELD, ALSO BRANDED TWIN LAKES] Note: material is welded carbon steel	AR027400ST	120 gal	Rigid base	2.00	2.40	UUT10b
	AR051201AJ	200 gal		2.00	2.40	Interpolated
	AR051301AJ	240 gal		2.00	2.40	UUT11bii
<b>Vertical tanks</b> [MANCHESTER TANK] Note: material is welded carbon steel (ASME, 165 PSIG)	AR063700AV	400 gal	Rigid base	2.00	2.40	UUT12c
	AR660000AV	660 gal		2.00	2.40	UUT15b
<b>Vertical tanks</b> [Morganton] Note: material is welded carbon steel	VES07285	80 gal	Rigid base	2.00	2.40	UUT 30a, 31a
	VES07387	80 gal				Interpolated
	VES04865	120 gal				Interpolated
	VES04767	120 gal				UUT 31a
	VES07303	200 gal				Interpolated
	VES07072	240 gal				UUT 30a
<b>Dew point monitor / probe desiccant</b> [POWEREX] Note: material of probe housing is stainless steel	PDPM1001AJ	N/A	Rigid base	2.00	2.40	UUT10b, UUT12b
	PDMP2001AJ	N/A		2.00	2.40	Extrapolated <sup>1</sup>
<b>Carbon monoxide monitor/ sensor</b> [ENMET] Note: material is FRP housing with circuit board and integrated sensor	03481-005	N/A	Rigid base	2.00	2.40	UUT10b, UUT12b
<b>Tank drain</b> [JORC] Note: material is cast brass body with integrated solenoid valve and DIN connector-mounted solid state timer	2523	Timer Drain	Rigid base	2.00	2.40	UUT10b
<b>Tank drain</b> [PARKER-DOMNICK HUNTER / ZANDER] Note: material is die cast body and molded polymer housing	ED3004N	No-Loss Drain	Rigid base	2.00	2.40	UUT15b

1. Extrapolated dew point monitor is the same as tested in UUT10b and UUT12b (software change only).

**Table 7 - Certified Subcomponents (Continued) - Stacked Units, Medical and Laboratory Scroll  
(Rigid Base Mount)**

Subcomponent [MFR]	Model	Dimensions (in)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
		Length	Width	Height					
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame, or powder coated carbon steel mounting platform.	PMD10	17	28	53	200	Rigid base	2.00	2.40	Extrapolated
	PMD17	17	28	53	200		2.00	2.40	Extrapolated
	PMD30	17	28	64	330		2.00	2.40	Extrapolated
	PMD35	17	28	64	330		2.00	2.40	Extrapolated
	PMD45	17	28	72	360		2.00	2.40	UUT10b
	PMD55	17	28	72	360		2.00	2.40	Interpolated
	PMD60	35	28	67	660		2.00	2.40	Interpolated
	PMD71	35	28	67	660		2.00	2.40	Interpolated
	PMD90	35	28	76	720		2.00	2.40	Interpolated
	PMD110	35	28	76	720		2.00	2.40	Interpolated
	PMD111	35	28	76	720		2.00	2.40	UUT 4b <sup>1</sup>
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame, or powder coated carbon steel mounting platform.	PLD10	17	28	53	200	Rigid base	2.00	2.40	Extrapolated
	PLD17	17	28	53	200		2.00	2.40	Extrapolated
	PLD30	17	28	64	330		2.00	2.40	Extrapolated
	PLD35	17	28	64	330		2.00	2.40	Extrapolated
	PLD45	17	28	72	360		2.00	2.40	UUT10b
	PLD55	17	28	72	360		2.00	2.40	Interpolated
	PLD60	35	28	67	660		2.00	2.40	Interpolated
	PLD71	35	28	67	660		2.00	2.40	Interpolated
	PLD90	35	28	76	720		2.00	2.40	Interpolated
	PLD111	35	28	76	720		2.00	2.40	UUT 4b <sup>1</sup>
<b>Desiccant dryers</b> [NANO PSI] Note: material is aluminum extruded towers; powder coated carbon steel mounting frame, or powder coated carbon steel mounting platform.	NDL110	17	13	48	172	Rigid base	2.00	2.40	Extrapolated
	NDL120	17	13	52	209		2.00	2.40	Extrapolated
	NDL130	17	13	56	262		2.00	2.40	UUT11bii
	NDL2110	25	12	47	366		2.00	2.40	UUT 9 <sup>2</sup>
<b>Desiccant dryers</b> [Trident] Note: material is aluminum extruded towers; powder coated carbon steel mounting frame, or powder coated carbon steel mounting platform.	PD204A	6	13	41	50	Rigid base	2.00	2.40	UUT 32
	PD205A	8	15	38	65		2.00	2.40	Interpolated
	PD206A	8	15	48	90		2.00	2.40	Interpolated
	PD207A	12	19	40	110		2.00	2.40	Interpolated
	PD208A	12	21	47	135		2.00	2.40	Interpolated
	PD209A	15	17	63	235		2.00	2.40	Interpolated
	PD210A	15	17	75	265		2.00	2.40	Interpolated
	PD211A	23	18	64	470		2.00	2.40	Interpolated
	PD212A	23	18	76	525		2.00	2.40	Interpolated
	PD213A	30	18	64	565		2.00	2.40	UUT 33i

Notes:

1. UUT 4b, which serves as the upper bookend, was tested on neoprene pads (see Table 7 continued)
2. UUT 9, which serves as the upper bookend, was tested on neoprene pads (see Table 7 continued)

**Table 8 - Certified Components - Rotary Tooth Oil Free Medical/Lab Air Systems**
**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Medical air model number	Lab air model number <sup>1</sup>	Hp	Vertical receiver gallons	Number of compressor enclosures	Number of compressors per enclosure	Maximum dimensions (in) <sup>2</sup>			Max. operating weight (lb) <sup>3</sup>	Mounting <sup>4</sup>	Sds (g), z/h=1	Fp/Wp	Unit
						Length	Width	Height					
Duplex Systems													
MDRC05074FA5	LDRC05072FA5	50 x 2	400	2	1	232	116	102	8,260	Rigid base w/ internal isolation	2.00	4.50	UUT12a,b,c <sup>5, 6</sup>
Triplex Systems													
MTRC05074FA5	LTRC05074KA5	50 x 3	400	3	1	332	116	102	11,190	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>7</sup>
Quadruplex Systems													
MQRC05074FA5	LQRC05074FA5	50 x 4	400	4	1	412	152	102	14,120	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>7</sup>
MQRC05084FA5	LQRC05084FA5	50 x 4	660	4	1	412	166	127	14,980	Rigid base w/ internal isolation	2.00	4.50	Extrapolated <sup>7</sup> with tank from UUT15b <sup>8</sup>

1. Lab units are physically identical to medical air units (software change only)

2. Dimensions include 24 inch spacing between system components. System component skids are independently mounted and flexibly connected.

3. Weight is sum of all system components

4. Compressor pump skids are internally isolated. Dryer and receiver tank skids are not.

5. Only one compressor enclosure tested in UUT12a (systems consist of 2 to 4 identical enclosures, independently mounted and flexibly connected)

6. Dimensions and weight shown here for the MDRC05074FA5 are calculated, assuming the duplex system contains two of the compressor enclosures tested in UUT12a, along with the dryer/controller and 400 gallon receiver tank tested in UUT12b and UUT12c.

7. Extrapolated units are the same as the unit tested, except with additional enclosures identical to that tested in UUT12a, all independently mounted and flexibly connected

8. Dimensions and weight shown here for the MQRC05084FA5 are calculated, assuming the quadruplex system contains four of the compressor enclosures tested in UUT12a, along with the dryer/controller tested in UUT12b and the 660 gallon receiver tank tested in UUT15b.

**Table 9 - Certified Subcomponents - Rotary Tooth Oil Free Medical/Lab Air Systems**

Subcomponent [MFR]	Model	Notes	Material	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
<b>Pump</b> [POWEREX]	PCCMD50074R2AJ	50 HP	Cast iron, w/ flange mounted motor. welded steel platform, bolted framing and sheet metal.	Rigid base w/ internal isolation	2.00	4.50	UUT12a
<b>Motor</b> [WEG]	03736ET3Y200L-W22	380/460V, 50 HP	Cast iron construction, flange mount	Rigid base w/ internal isolation	2.00	4.50	UUT12a
<b>Aftercooler</b> [POWEREX]	Custom	50 HP aftercooler, intercooler and oil cooler integrated into compressor package design	Aluminum	Rigid base w/ internal isolation	2.00	4.50	UUT12a
<b>Intake filter elements</b> [MANN]	45 402 92 960	PCC and PCCMD	Molded polymer	Rigid base w/ internal isolation	2.00	4.50	UUT12a
<b>Check valves</b> [POWEREX]	Custom	Check valve integrated into PCC compressor unit	Cast Iron	Rigid base w/ internal isolation	2.00	4.50	UUT12a
<b>Vertical tanks</b> [MANCHESTER TANK]	AR063700AV	400 gal	Welded carbon steel (ASME, 165 PSIG)	Rigid base	2.00	2.40	UUT12c
	AR660000AV	660 gal	Welded carbon steel (ASME, 165 PSIG)	Rigid base	2.00	2.40	UUT15b
<b>Controllers</b> <sup>1</sup> [POWEREX]	PXTM215X1AJ	208-230V / 460V, Duplex 50 HP	Painted carbon steel electrical cabinet, NEMA 12	Rigid base	2.00	2.40	Extrapolated
	PXTM218AXAJ	208-230V / 460V, Duplex 50 HP	Painted carbon steel electrical cabinet, NEMA 12	Rigid base	2.00	2.40	UUT14b
	PXTM315X1AJ	208-230V / 460V, Triplex 50 HP	Painted carbon steel electrical cabinet, NEMA 12	Rigid base	2.00	2.40	Interpolated
	PXTM415X1AJ	208-230V / 460V, Quadruplex 50 HP	Painted carbon steel electrical cabinet, NEMA 12	Rigid base	2.00	2.40	UUT12b
<b>Tank Drain</b> [JORC]	3623-UL, 3622	No-loss drain; Smart Guard or Smart Guard Mini	Die cast body and molded polymer housing	Rigid base	2.00	2.40	UUT12c, UUT15b
<b>Desiccant dryers</b> [NANO PSI]	NDL2120	16"Lx25"Wx61"H, 450 lb	Aluminum extruded towers; powder coated carbon steel mounting frame	Rigid base	2.00	2.40	UUT12b
	NDL2130	16"Lx25"Wx75"H, 750 lb		Rigid base	2.00	2.40	Interpolated
	NDL3130	16"Lx31"Wx75"H, 800 lb		Rigid base	2.00	2.40	Interpolated
	NDL4130	16"Lx38"Wx75"H, 1160 lb		Rigid base	2.00	2.40	UUT12b

1. Controllers are universal voltage design. Each controller operates compressors of any voltage (208-230V / 460V) and requires 120 VAC input.

**Table 10 - Certified Components - Scroll Enclosed (SE) Medical/Laboratory Air Systems**

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

Medical air model number <sup>1</sup>	Lab air model number <sup>1,2</sup>	Hp per pump	Total Hp	Vertical receiver (gallons)	Number of compressor enclosures	Vertically stacked pumps per enclosure	Horizontally arrayed pumps per enclosure	Maximum Dimensions (in)			Max. operating weight (lb)	Mounting <sup>3</sup>	Sds (g), z/h=1	Fp/Wp	Unit
								Length	Width	Height					
Duplex systems (individual enclosed compressor units with structurally independent and flexibly attached a tank/dryer/control skids)															
MSED1003x5	LSED1003x5	5	10 x 2	80	2	2	1	94	80	71	2,650	Rigid base w/ internal isolation	2.00	4.50	Extrapolated
MSED1504x5	LSED1504x5	5	15 x 2	120	2	3	1	94	80	79	2,980		2.00	4.50	Extrapolated
MSED2004x5 <sup>1</sup>	LSED2004x5	5	20 x 2	120	2	4	1	94	80	79	3,280		2.00	4.50	UUT14a,b <sup>4</sup>
MSED2005x5	LSED2005x5	5	20 x 2	200	2	4	1	94	80	84	3,380		2.00	4.50	Interpolated
MSED3006x5	LSED3006x5	5	30 x 2	240	2	3,3	2	95	140	96	5,100		2.00	4.50	Interpolated
MSED4006x5	LSED4006x5	5	40 x 2	240	2	4,4	2	95	140	96	5,500		2.00	4.50	Interpolated
MSED15B4x5	LSED15B4x5	7.5	15 x 2	120	2	2	1	99	104	79	3,050		2.00	4.50	Interpolated
MSED20B4x5	LSED20B4x5	10	20 x 2	120	2	2	1	99	104	79	3,170		2.00	4.50	Interpolated
MSED22B4x5	LSED22B4x5	7.5	22.5 x 2	120	2	3	1	99	104	79	4,000		2.00	4.50	Interpolated
MSED30B5x5	LSED30B5x5	10	30 x 2	200	2	3	1	99	104	84	4,700		2.00	4.50	Interpolated
MSED50B6x5	LSED50B6x6	10	50 x 2	240	2	2,3	2	99	165	96	5,600	2.00	4.50	Interpolated	
Triplex systems (individual enclosed compressor units with a tank/dryer/control skid)															
MSET1004x5	LSET1004x5	5	10 x 3	120	3	2	1	95	125	79	3,550	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSET1505x5	LSET1505x5	5	15 x 3	200	3	3	1	95	125	84	4,750		2.00	4.50	Interpolated
MSET2005x5	LSET2005x5	5	20 x 3	200	3	4	1	95	125	84	4,800		2.00	4.50	Interpolated
MSET2006x5	LSET2006x5	5	20 x 3	240	3	4	1	95	125	96	4,900		2.00	4.50	Interpolated
MSET3006x5	LSET3006x5	5	30 x 3	240	3	3,3	1	96	223	96	6,500		2.00	4.50	Interpolated
MSET4006x5	LSET4006x5	5	40 x 3	240	3	4,4	2	96	223	96	8,200		2.00	4.50	Interpolated
MSET20B6x5	LSET20B6x5	10	20 x 3	240	3	2	1	99	175	96	4,052		2.00	4.50	Interpolated
MSET2256x5	LSET2256x5	7.5	22.5 x 3	240	3	3	1	99	175	96	4,850		2.00	4.50	Interpolated
MSET30B6x5	LSET30B6x5	10	30 x 3	240	3	3	1	99	175	96	6,550		2.00	4.50	Interpolated
MSET40B6x5	LSET40B6x5	10	40 x 3	240	3	2,2	2	99	259	96	7,316		2.00	4.50	Interpolated
MSET50B7x5	LSET50B7x5	10	50 x 3	400	3	2,3	2	99	259	96	8,552		2.00	4.50	Interpolated
MSET60B7x5	LSET60B7x5	10	60 x 3	400	3	3,3	2	99	259	96	9,452		2.00	4.50	Interpolated

Continued on Next Page

1. In model numbers listed, the "x" can be 2 = 208V, 3 = 230V, or 4 = 460V. UUT14a,b was MSED200425 (208V) and UUT15a,b was LSEQ60B845 (460V).

2. Lab units are physically identical to medical air units (software change only)

3. Compressor pump skids are internally isolated. Dryer and receiver tank skids are not.

4. Dimensions and weight shown here for the MSED2004xx system are calculated, assuming the duplex system contains two of the compressor enclosures tested in UUT14a, along with a skid containing a controller, tank, dryers, and other subcomponents as shown in the Scroll Enclosed certified subcomponent tables.

**Table 10 - Certified Components (Continued) - Scroll Enclosed (SE) Medical/Laboratory Air Systems**


Medical air model number <sup>1</sup>	Lab air model number <sup>1,2</sup>	Hp per pump	Total Hp	Vertical receiver (gallons)	Number of compressor enclosures	Vertically stacked pumps per enclosure	Horizontally arrayed pumps per enclosure	Maximum Dimensions (in)			Max. operating weight (lb)	Mounting <sup>3</sup>	Sds (g), z/h=1	Fp/Wp	Unit
								Length	Width	Height					
Quadruplex systems (individual enclosed compressor units with a tank/dryer/control skid)															
MSEQ1505x5	LSEQ1505x5	5	15 x 4	200	4	3	1	132	100	84	5,050	Rigid base w/ internal isolation	2.00	4.50	Interpolated
MSEQ2006x5	LSEQ2006x5	5	20 x 4	240	4	4	1	132	100	96	6,150		2.00	4.50	Interpolated
MSEQ3007x5	LSEQ3007x5	5	30 x 4	400	4	3, 3	2	212	126	109	8,730		2.00	4.50	Interpolated
MSEQ4007x5	LSEQ4007x5	5	40 x 4	400	4	4, 4	2	212	126	109	9,890		2.00	4.50	Interpolated
MSEQ2256x5	LSEQ2256x5	7.5	22.5 x 4	240	4	3	1	99	246	96	5,900		2.00	4.50	Interpolated
MSEQ30B6x5	LSEQ30B6x5	10	30 x 4	240	4	3	1	99	246	96	6,400		2.00	4.50	Interpolated
MSEQ40B6x5	LSEQ40B6x5	10	40 x 4	240	4	2, 2	2	220	122	96	9,400		2.00	4.50	Interpolated
MSEQ40B7x5	LSEQ40B7x5	10	40 x 4	400	4	2, 2	2	220	122	102	10,100		2.00	4.50	Interpolated
MSEQ45B8x5	LSEQ45B8x5	7.5	45 x 4	660	4	3, 3	2	220	122	127	11,700		2.00	4.50	Interpolated
MSEQ50B8x5	LSEQ50B8x5	10	50 x 4	660	4	2, 3	2	220	122	127	11,800		2.00	4.50	Interpolated
MSEQ60B8x5 <sup>1</sup>	LSEQ60B8x5	10	60 x 4	660	4	3, 3	2	220	150	127	13,200	2.00	4.50	UUT15a,b <sup>4</sup>	

1. In model numbers listed, the "x" can be 2 = 208V, 3 = 230V, or 4 = 460V. UUT14a,b was MSED200425 (208V) and UUT15a,b was LSEQ60B845 (460V).

2. Lab units are physically identical to medical air units (software change only)

3. Compressor pump skids are internally isolated. Dryer and receiver tank skids are not.

4. Dimensions and weight shown here for the MSEQ60B8x5 system are calculated, assuming the quadruplex system contains four of the compressor enclosures tested in UUT15a, one 660 gallon tank as tested in UUT15b, and a skid containing a controller, dryers, and other subcomponents as shown in the Scroll Enclosed certified subcomponent tables.

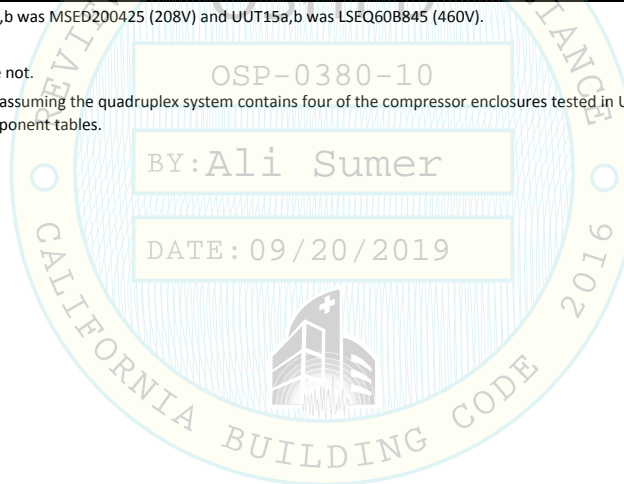



**Table 11 - Certified Subcomponents - Scroll Enclosed (SE) Medical/Laboratory Air Systems**

Subcomponent [MFR]	Model	Notes	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
<b>Scroll pumps</b> [POWEREX]  Note: material is die cast aluminum. Pump motor assemblies mounted in welded and bolted steel frame with enclosing sheet metal Note: Pumps are belt driven	SED1007	5 Hp (2)	Rigid base w/ internal isolation	2.00	4.50	Extrapolated
	SET1507	5 Hp (3)		2.00	4.50	Extrapolated
	SEQ2007	5 Hp (4)		2.00	4.50	UUT14a
	SEH3007	5 Hp (6)		2.00	4.50	Interpolated
	SEO4007	5 Hp (8)		2.00	4.50	Interpolated
	SED15B7	7.5 Hp (2)		2.00	4.50	Interpolated
	SED20B7	10 Hp (2)		2.00	4.50	Interpolated
	SET2257	7.5 Hp (3)		2.00	4.50	Interpolated
	SET30B7	10 Hp (3)		2.00	4.50	Interpolated
	SEQ40B7	10 Hp (4)		2.00	4.50	Interpolated
	SEP50B7	10 Hp (5)		2.00	4.50	Interpolated
	SEH45B7	7.5 Hp (6)		2.00	4.50	Interpolated
	SEH60B7	10 Hp (6)		2.00	4.50	UUT15a
<b>Motors</b> [WEG]  Note: material is TEFC design, carbon steel shell w/ welded foot	00518ET3E184T-SRT	208-230V / 460V, 5 Hp	Rigid base w/ internal isolation	2.00	4.50	UUT14a
	00736ET3E213T-S	208-230V / 460V, 7.5 Hp		2.00	4.50	Interpolated
	01036ET3E215T-S	208-230V / 460V, 10 Hp		2.00	4.50	UUT15a
<b>Check valve</b> [POWEREX] Note: material is aluminum (anodized body), in-line design	Custom	Check valve for 5, 7.5, and 10 HP scroll compressors in enclosures	Rigid base w/ internal isolation	2.00	4.50	UUT14a, UUT15a
<b>Controllers</b> [POWEREX] Note: material is painted carbon steel electrical cabinet Note: lower case "x" in model number is 4 for 460V, 3 for 230V, and 2 for 208V	HMI_PXMI	NEMA 12 enclosure: Human Machine Interface: Touchscreen	Rigid base w/ internal isolation	2.00	4.50	Extrapolated
	PBMI_PXMI	NEMA 12 enclosure: Powerex Building Management Integrator: HMI panel w/ additional communications card		2.00	4.50	UUT10a, UUT11aii
Continued on Next Page						

**Table 11 - Certified Subcomponents (Continued) - Scroll Enclosed (SE) Medical/Laboratory Air Systems**

Subcomponent [MFR]	Model	Notes	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
<b>Controllers</b> [POWEREX]  Note: material is painted carbon steel electrical cabinet Note: lower case "x" in model number is 4 for 460V, 3 for 230V, and 2 for 208V	PXEM218AxAJ	NEMA 12 enclosure, 10 HP duplex	Rigid base	2.00	2.40	UUT14b
	PXEM218FxAJ	NEMA 12 enclosure, 15 HP duplex		2.00	2.40	Interpolated
	PXEM218GxAJ	NEMA 12 enclosure, 20 HP duplex		2.00	2.40	Interpolated
	PXEM218IxAJ	NEMA 12 enclosure, 30 HP duplex		2.00	2.40	Interpolated
	PXEM218KxAJ	NEMA 12 enclosure, 40 HP duplex		2.00	2.40	Interpolated
	PXEM215XxAJ	NEMA 12 enclosure, 22.5-60 HP duplex		2.00	2.40	Interpolated
	PXEM318AxAJ	NEMA 12 enclosure, 10 HP triplex		2.00	2.40	Interpolated
	PXEM318FxAJ	NEMA 12 enclosure, 15 HP triplex		2.00	2.40	Interpolated
	PXEM318GxAJ	NEMA 12 enclosure, 20 HP triplex		2.00	2.40	Interpolated
	PXEM318IxAJ	NEMA 12 enclosure, 30 HP triplex		2.00	2.40	Interpolated
	PXEM318KxAJ	NEMA 12 enclosure, 40 HP triplex		2.00	2.40	Interpolated
	PXEM315XxAJ	NEMA 12 enclosure, 22.5-60 HP triplex		2.00	2.40	Interpolated
	PXEM418AxAJ	NEMA 12 enclosure, 10 HP quadruplex		2.00	2.40	Interpolated
	PXEM418FxAJ	NEMA 12 enclosure, 15 HP quadruplex		2.00	2.40	Interpolated
	PXEM418GxAJ	NEMA 12 enclosure, 20 HP quadruplex		2.00	2.40	Interpolated
	PXEM418IxAJ	NEMA 12 enclosure, 30 HP quadruplex		2.00	2.40	Interpolated
	PXEM418KxAJ	NEMA 12 enclosure, 40 HP quadruplex		2.00	2.40	UUT14b
	PXEM415XxAJ	NEMA 12 enclosure, 22.5-60 HP quadruplex		2.00	2.40	UUT12b
<b>Vertical tanks</b> [CAMPBELL HAUSFELD, ALSO BRANDED TWIN LAKES] Note: material is welded carbon steel	AR027400ST	120 gal	Rigid base	2.00	2.40	UUT10b
	AR051201AJ	200 gal		2.00	2.40	Interpolated
	AR051301AJ	240 gal		2.00	2.40	UUT11bii
<b>Vertical tanks</b> [MANCHESTER TANK] Note: material is welded carbon steel, ASME 165 PSIG	AR063700AV	400 gal	Rigid base	2.00	2.40	UUT12c
	AR660000AV	660 gal		2.00	2.40	UUT15b
<b>Vertical tanks</b> [Morganton] Note: material is welded carbon steel	VES07285	80 gal	Rigid base	2.00	2.40	UUT 30a, 31a
	VES04865	120 gal				Interpolated
	VES04767	120 gal				UUT 31a
	VES07303	200 gal				Interpolated
	VES07072	240 gal				UUT 30a

**Table 11 - Certified Subcomponents (Continued) - Scroll Enclosed (SE) Medical/Laboratory Air Systems**

Subcomponent [MFR]	Model	Dimensions (in)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
		Length	Width	Height					
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame, or powder coated carbon steel mounting platform.	PMD10	17	28	53	200	Rigid base	2.00	2.40	Extrapolated
	PMD17	17	28	53	200		2.00	2.40	Extrapolated
	PMD30	17	28	64	330		2.00	2.40	Extrapolated
	PMD35	17	28	64	330		2.00	2.40	Extrapolated
	PMD45	17	28	72	360		2.00	2.40	UUT10b
	PMD55	17	28	72	360		2.00	2.40	Interpolated
	PMD60	35	28	67	660		2.00	2.40	Interpolated
	PMD71	35	28	67	660		2.00	2.40	Interpolated
	PMD90	35	28	76	720		2.00	2.40	Interpolated
	PMD110	35	28	76	720		2.00	2.40	Interpolated
	PMD111	35	28	76	720		2.00	2.40	UUT 4b <sup>1</sup>
<b>Desiccant dryers</b> [POWEREX]  Note: material is powder coated welded carbon steel tanks; powder coated welded carbon steel mounting frame, or powder coated carbon steel mounting platform.	PLD10	17	28	53	200	Rigid base	2.00	2.40	Extrapolated
	PLD17	17	28	53	200		2.00	2.40	Extrapolated
	PLD30	17	28	64	330		2.00	2.40	Extrapolated
	PLD35	17	28	64	330		2.00	2.40	Extrapolated
	PLD45	17	28	72	360		2.00	2.40	UUT10b
	PLD55	17	28	72	360		2.00	2.40	Interpolated
	PLD60	35	28	67	660		2.00	2.40	Interpolated
	PLD71	35	28	67	660		2.00	2.40	Interpolated
	PLD90	35	28	76	720		2.00	2.40	Interpolated
	PLD111	35	28	76	720		2.00	2.40	UUT 4b <sup>1</sup>
<b>Desiccant dryers</b> [NANO PSI]  Note: material is aluminum extruded towers; powder coated carbon steel mounting frame, or powder coated carbon steel mounting platform.	NDL110	17	13	48	172	Rigid base	2.00	2.40	Extrapolated
	NDL120	17	13	52	209		2.00	2.40	Extrapolated
	NDL130	17	13	56	262		2.00	2.40	UUT11bii
	NDL2110	25	12	47	366		2.00	2.40	Interpolated
	NDL2120	16	25	61	450		2.00	2.40	UUT12b
	NDL2130	16	25	75	750		2.00	2.40	Interpolated
	NDL3130	16	31	75	800		2.00	2.40	Interpolated
	NDL4130	16	38	75	1160		2.00	2.40	UUT12b

Notes:  
 1. UUT 4b, which serves as the upper bookend, was tested on neoprene pads (see Table 7 continued)

**Table 12 - Certified Components - Medical Gas Automatic Changeover Manifolds**
**Manufacturer:** Powerex (alternately branded Tri-Tech Medical)

**Product Line:** Medical Gas Automatic Changeover Manifolds

Powerex Model Number <sup>1,2,3</sup>	Tri-Tech Medical Model Number	Control	Gas Containers <sup>4</sup>	Cabinet	Delivery Pressure (psi)	Dimensions (inches)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
						Width	Depth	Height					
PX-NPCU12AI1L	NPCU12AI1L	Analog	C x C	Standard	50	15	9	25	66	Rigid wall	2.00	1.50	UUT28
PX-NPCU12xxxL	NPCU12xxxL	Analog	C x C	Standard	50, 80 or 170	15	9	25	66 to 70	Rigid wall	2.00	1.50	Interpolated
PX-NPCU12xxxH	NPCU12xxxH	Analog	C x C	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-NPCU22xxxL	NPCU22xxxL	Analog	C x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-NPCU22xxxH	NPCU22xxxH	Analog	C x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-CCU12xxxL	CCU12xxxL	Digital	C x C	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-CCU12xxxH	CCU12xxxH	Digital	C x C	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-CCU22xxxL	CCU22xxxL	Digital	C x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-CCU22xxxH	CCU22xxxH	Digital	C x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-PLU12xxxL	PLU12xxxL	Digital	L x C	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-PLU12xxxH	PLU12xxxH	Digital	L x C	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-PLU22xxxL	PLU22xxxL	Digital	L x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-PLU22xxxH	PLU22xxxH	Digital	L x C	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-LLU12xxxL	LLU12xxxL	Digital	L x L	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-LLU12xxxH	LLU12xxxH	Digital	L x L	Standard		15	9	25		Rigid wall	2.00	1.50	Interpolated
PX-LLU22xxxL	LLU22xxxL	Digital	L x L	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-LLU22xxxH	LLU22xxxH	Digital	L x L	Weatherproof		19	11	27		Rigid wall	2.00	1.50	Interpolated
PX-LLU22NT3H	LLU22NT3H	Digital	L x L	Weatherproof	170	19	11	27	70	Rigid wall	2.00	1.50	UUT29

1. First and second lower case "x" in model number stand for medical gas type: AI=medical air, CD=carbon dioxide, IA=instrument air, NT=Nitrogen, NO=nitrous oxide, OX=oxygen, AR=argon

2. Third lower case "x" in model number stands for delivery pressure in psi: 1=50, 2=80, 3=170

3. Last digit in model number stands for Flow: L = Standard Flow; H = High Flow

4. Gas Containers: C x C = Cylinder x Cylinder; L x L = Liquid x Liquid; L x C = Liquid x Cylinder

**Table 13 - Certified Subcomponents - Medical Gas Automatic Changeover Manifolds**

Model	Manufacturer	Description	Material	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
PT	Tri-Tech Medical	Standard Enclosure	Powder-coated carbon steel, NEMA 1	Rigid wall	2.0	1.50	UUT28
PLU	Tri-Tech Medical	Weatherproof Enclosure	Powder-coated carbon steel, NEMA 1	Rigid wall	2.0	1.50	UUT29
PX-68-0003R	Victor	Primary regulator	Brass	Rigid wall	2.0	1.50	UUT28
PX-68-0017R	Harris	Line regulator standard flow 5-125 psig	Brass	Rigid wall	2.0	1.50	UUT28
PX-68-0004R	Harris	Line regulator standard flow 5-125 psig	Brass	Rigid wall	2.0	1.50	UUT29
PX-68-0002R	Victor	Line regulator high flow 5-125 psig	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-68-0001R	Victor	Line regulator high flow 10-200 psig	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-35-1007R	IDC	Circuit board	Phenolic and electrical components	Rigid wall	2.0	1.50	UUT28
PX-35-1003R	IDC	Circuit board	Phenolic and electrical components	Rigid wall	2.0	1.50	Interpolated
PX-35-1004R	IDC	Circuit board	Phenolic and electrical components	Rigid wall	2.0	1.50	UUT29
PX-35-2013R	Hughes Peters	Power supply	Various including copper and stainless steel	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-3001R	Measurement Specialties	0-2500 psig transducer w/ 3' cable for left or right banks	Stainless steel housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3024	Tri-Tech Medical	0-250 psig transducer w/ 1.5' cable N2	Aluminum housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3025	Tri-Tech Medical	0-100 psig transducer w/ 1.5' cable Oxy	Aluminum housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3026	Tri-Tech Medical	0-100 psig transducer w/ 1.5' cable Med Air	Aluminum housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3027	Tri-Tech Medical	0-100 psig transducer w/ 1.5' cable N2O	Aluminum housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3028	Tri-Tech Medical	0-100 psig transducer w/ 1.5' cable CO2	Aluminum housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3001-12R	Tri-Tech Medical	0-2500 psig transducer w/ 12' cable for emergency reserve low	Stainless steel housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3001-5R	Tri-Tech Medical	0-2500 psig transducer w/ 15' cable for right bank low	Stainless steel housing, internal electronics	Rigid wall	2.0	1.50	UUT29
PX-14-3002	Measurement Specialties	0-500 psig transducer w/ 3' cable for left or right banks and emergency reserve in use	Stainless steel housing, internal electronics	Rigid wall	2.0	1.50	UUT29

**Table 13 - Certified Subcomponents (Continued) - Medical Gas Automatic Changeover Manifolds**

Model	Manufacturer	Description	Material	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
PX-14-2013	United Electric	Left bank pressure switch	Plastic, stainless steel & brass	Rigid wall	2.0	1.50	UUT28
PX-14-2014	United Electric	Right bank pressure switch	Plastic, stainless steel & brass	Rigid wall	2.0	1.50	UUT28
PX-48-1007R	TTM	Solenoid Valve	Brass	Rigid wall	2.0	1.50	UUT28
PX-48-1008R	TTM	Left Solenoid Valve for LLU/PLU	Brass	Rigid wall	2.0	1.50	UUT29
PX-48-1009R	TTM	Right Solenoid Valve for LLU/PLU	Brass	Rigid wall	2.0	1.50	UUT29
PX-17-4003R	TTM	Intermediate check valve 1/2" NPT male x 1/2" OD tube	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-1018	WIKA	0-4000 psig 1-1/2" x 1/8" M NPT center back gage	Plastic & brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-1016	WIKA	0-400 psig 2" x 1/4" M NPT bottom port gage	Plastic & brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-1017	WIKA	0-400 psig 1-1/2" x 1/8" M NPT center back gage	Plastic & brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-1009	WIKA	0-300 psig 1-1/2" x 1/8" M NPT center back gage	Plastic & brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-14-1008	WIKA	0-100 psig 1-1/2" x 1/8" M NPT center back gage	Plastic & brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-RV-22-075	Rego	75 psig x 1/2" M NPT inlet w/ pipe away adapt	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-RV-22-150	Rego	150 psig x 1/2" M NPT inlet w/ pipe away adapt	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-RV-22-250	Rego	250 psig x 1/2" M NPT inlet w/ pipe away adapt	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-RV-11-400	Rego	400 psig x 1/4" M NPT inlet w/ pipe away adapt	Brass	Rigid wall	2.0	1.50	UUT28, UUT29
PX-17-0169	Fairview Fittings	Union 3 piece 1/2" M NPT x 1/2" M NPT 1" 11-1/2 NPS	Brass	Rigid wall	2.0	1.50	UUT28, UUT29



Table 14 - Tested Units

Manufacturer: Powerex

Product Line: Medical Air and Laboratory Air

Type	Model number	Total number of pumps	Vertically stacked pumps or layers	Horizontally arrayed pumps	Dimensions (inches)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
					Length	Width	Height					
Stacked Units  1. Note: Indicated length and/or height are combined overall dimensions for the individual unit skids	MSD02034L5	2	2	1	50.0	31.0	78.0	1,040	Flexible base (neoprene), w/ internal isolation	2.50	4.50	UUT1
	LSD02034L5	2	2	1	74.0	32.0	62.0	1,090	Flexible base (neoprene), w/ internal isolation	2.50	4.50	UUT2
	MSQ05044P5	4	4	1	77.4	32.0	77.0	1,870	Flexible base (neoprene), w/ internal isolation	2.50	4.50	UUT3
	MSD15064L5 (controller/pump skid)	6	2	3	84 <sup>1</sup>	34.0	96 <sup>1</sup>	1,510	Flexible base (neoprene), w/ internal isolation	2.50	4.50	UUT4a
	MSD15064L5 (receiver/dryer skid)	N/A	N/A	N/A		32.0		1,310	Flexible base (neoprene)	2.42	4.36	UUT4b
	MSQ15064L5 (controller/pump skid)	12	3	4	108 <sup>1</sup>	34.0	96 <sup>1</sup>	2,950	Flexible base (neoprene), w/ internal isolation	2.00	3.60	UUT7
	MSQ15064L5 (receiver/dryer skid)	N/A	N/A	N/A		32.0		1,310	Flexible base (neoprene)	2.42	4.36	UUT5b
	Dryer skid	N/A	N/A	N/A	98.0	32.0	79.0	965	Flexible base (neoprene)	2.42	4.36	UUT6
	MSD15B44K5 (controller/pump skid)	4	4	1	61 <sup>1</sup>	32.5	78 <sup>1</sup>	1,550	Rigid base, w/ internal isolation	2.00	4.50	UUT10a
	MSD15B44K5 (receiver/dryer skid)	N/A	N/A	N/A		33.5		840	Rigid base	2.00	2.40	UUT10b
	MSQ20B62P5 (controller/pump skid)	8	7	2	79 <sup>1</sup>	33.5	93 <sup>1</sup>	3,120	Rigid base, w/ internal isolation	2.00	4.50	UUT11aii
	MSQ20B62P5 (receiver/dryer skid)	N/A	N/A	N/A		43.0		1,680	Rigid base	2.00	2.40	UUT11bii
	Dryer skid (NDL110 and NDL2110 dryers)	N/A	N/A	N/A	55.0	31.5	67.0	800	Flexible base (neoprene)	2.00	3.60	UUT9
	MSD02A3	2	2	N/A	50.5	30.5	75.0	1,060	Rigid base, w/ internal isolation	2.00	4.50	UUT 32
	MSP15A6 (receiver/dryer/controller skid)	N/A	N/A	N/A	86.0	34.0	91.0	2,110	Rigid base	2.00	2.40	UUT 33i
	MSP15A6 (pump skid)	15	2,3	3	86.0	34.0	80.0	4,030	Rigid base, w/ internal isolation	2.00	4.50	UUT 33ii
Rotary Tooth Oil Free Medical Air Systems	MDRC05074FA5 (pump skid)	1	1	1	77.5	39.4	65.2	2,930	Rigid base, w/ internal isolation	2.00	4.50	UUT12a
	MDRC05074FA5 (dryer/controller skid)	N/A	N/A	N/A	32.0	99.2	80.3	1,760	Rigid base	2.00	2.40	UUT12b
	MDRC05074FA5 (400 gallon receiver tank)	N/A	N/A	N/A	38.2	47.2	101.5	640	Rigid base	2.00	2.40	UUT12c
Scroll Enclosed Compressed Air Systems  Note: compressor enclosures are structurally independent and flexibly connected. Only one compressor enclosure tested in each UUT14a and UUT15a.	MSED200425 (pump skid)	4	4	1	46.4	35.2	61.2	1,030	Rigid base, w/ internal isolation	2.00	4.50	UUT14a
	MSED200425 (controller skid); 2 controllers tested: PXEM218G2AJ and PXEM418G2AJ	N/A	N/A	N/A	55.0	39.8	79.4	560	Rigid base	2.00	2.40	UUT14b
	LSEQ60B845 (pump skid)	6	3,3	2	51.0	73.8	61.2	2,740	Rigid base, w/ internal isolation	2.00	4.50	UUT15a
	LSEQ60B845 (660 gallon receiver tank)	N/A	N/A	N/A	42.0	42.0	126.5	1,500	Rigid base	2.00	2.40	UUT15b
Miscellaneous	Platform base, 80 gallon vertical tank, 240 gallon vertical tank	N/A	N/A	N/A	33.5	60.0	94.0	1,010	Rigid base	2.00	2.40	UUT 30a
	Platform base, 80 gallon vertical tank, 240 gallon vertical tank	N/A	N/A	N/A	33.5	60.0	94.0	1,010	Flexible base (neoprene)	2.00	3.60	UUT 30b
	Ladder Frame base, 80 gallon vertical tank, 120 gallon vertical tank	N/A	N/A	N/A	32.0	55.0	75.0	630	Rigid base	2.00	2.40	UUT 31a
	Ladder Frame base, 80 gallon vertical tank, 120 gallon vertical tank	N/A	N/A	N/A	32.0	55.0	75.0	630	Flexible base (neoprene)	2.00	3.60	UUT 31b

**Table 14 - Tested Units (Continued)**


**Manufacturer:** Powerex

**Product Line:** Medical Gas Automatic Changeover Manifolds

Type	Powerex Model	Tri-Tech Medical Model	Control	Gas Container Type	Cabinet	Delivery Pressure	Flow	Dimensions (inches)			Weight (lb)	Mounting	Sds (g), z/h=1	Fp/Wp	Unit
								Depth	Width	Height					
Medical Gas Automatic Changeover Manifolds (Alternately Branded Tri-Tech Medical)	PX-NPCU12AI1L	NPCU12AI1L	Analog	C x C	Standard	50 PSIG	L	9	15	25	66	Rigid wall	2.00	1.50	UUT28
	PX-LLU22NT3H	LLU22NT3H	Digital	L x L	Weatherproof	170 PSIG	H	11	19	27	70	Rigid wall	2.00	1.50	UUT29

C x C = Cylinder x Cylinder, and L x L = Liquid x Liquid

Flow: L = Standard Flow; H = High Flow

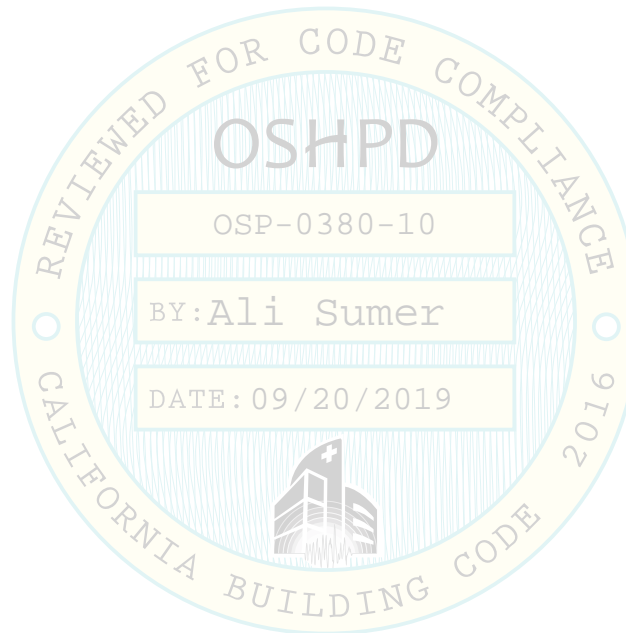

# UUT1

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSD02034L5

**Product Construction Summary:** Powder coated structural steel skid and frame. Unit is internally isolated.

### Options / Component Summary:

2HP scroll pump with WEG motor, 80 gallon vertical receiver tank, dew point monitor, CO monitor, BASIC\_PSM controller in NEMA 12 enclosure, timer drain, aftercooler, intake filter element, check valve, and PMD07T desiccant air dryer.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,040	UUT1	50	31	78	6.3	5.8	24.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.50	1.0	1.5	4.00	3.00	1.67	0.67

### Unit Mounting Description:



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 3/8"-diameter, Grade 5 bolts and washers spaced at approximately 30" widthwise and 48" lengthwise on center.

## UUT2

### UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** LSD02034L5

**Product Construction Summary:** Powder coated structural steel skid and frame. Unit is internally isolated.

**Options / Component Summary:**

2HP scroll pump with WEG motor, 80 gallon vertical receiver tank, dew point monitor, CO monitor, PBMI\_PXMI controller in NEMA 12 enclosure, no-loss drain, aftercooler, intake filter element, check valve, and KMT3 desiccant air dryer.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,090	UUT2	74	32	62	8.8	8.0	13.5

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.50	1.0	1.5	4.00	3.00	1.67	0.67

**Unit Mounting Description:**



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 31" widthwise and 72" lengthwise on center.



# UT3

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSQ05044P5

**Product Construction Summary:** Powder coated structural steel skid and frame. Unit is internally isolated.

**Options / Component Summary:**

5HP scroll pump with WEG motor, 120 gallon vertical receiver tank, dew point monitor, CO monitor, PBMI\_PXMI controller in NEMA 12 enclosure, timer drain, aftercooler, intake filter element, check valve, and PMD30 desiccant air dryer.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,870	UUT3	77	32	77	6.5	5.0	14.5

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.50	1.0	1.5	4.00	3.00	1.67	0.67

### Unit Mounting Description:



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 31" widthwise and 75" lengthwise on center.

# UUT4a

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSD15064L5 (controller/pump skid)

**Product Construction Summary:** Powder coated structural steel skid and frame. Unit is internally isolated.

### Options / Component Summary:

5HP scroll pump with WEG motor, dew point monitor, CO monitor, PBMI\_PXMI controller in NEMA 12 enclosure, timer drain, aftercooler, intake filter element and check valve.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties


Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,510	UUT4a	84*	34	96*	6.8	5.5	12.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.50	1.0	1.5	4.00	3.00	1.67	0.67

\*Note: Length and height are combined dimensions for UUT4a and UUT4b.

### Unit Mounting Description:

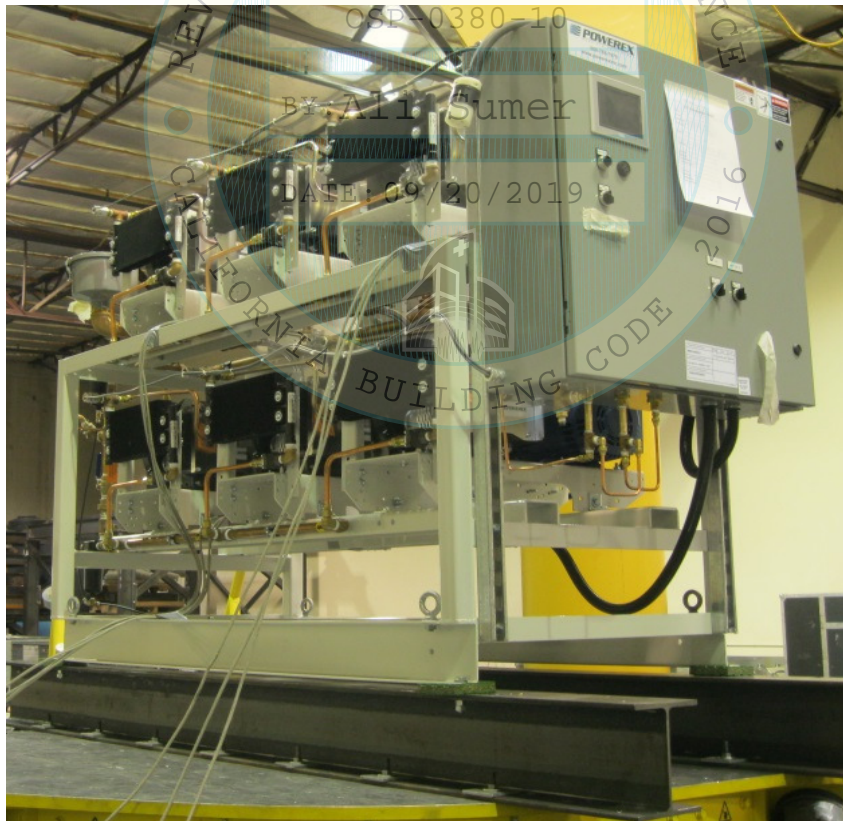

The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced approximately 32" widthwise and 74" lengthwise on center.



**UUT4b****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** MSD15064L5 (receiver/dryer skid)**Product Construction Summary:** Powder coated structural steel skid and frame**Options / Component Summary:**

240 gallon vertical receiver tank and PMD111 desiccant air dryer.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,310	UUT4b	84*	32	96*	5.5	5.0	22.5

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.42	1.0	1.5	3.87	2.90	1.61	0.65

\*Note: Length and height are combined dimensions for UUT4a and UUT4b.

**Unit Mounting Description:**

The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced approximately 30" widthwise and 74" lengthwise on center.

# UUT5b

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSQ15064L5 (receiver/dryer skid)

**Product Construction Summary:** Powder coated structural steel skid and frame

**Options / Component Summary:**

240 gallon vertical receiver tank and DME050RX desiccant air dryer.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,310	UUT5b	108*	32	96*	6.3	5.5	17.5

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.42	1.0	1.5	3.87	2.90	1.61	0.65

\*Note: Length and height are combined dimensions for UUT7 and UUT5b.

### Unit Mounting Description:



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced approximately 30" widthwise and 78" lengthwise on center.

**UUT6****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** Desiccant air dryers KMT4, DME015, DME060 and DME080RX**Product Construction Summary:** Powder coated structural steel skid and frame**Options / Component Summary:** KMT4, DME015, DME060 and DME080RX desiccant air dryers**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
965	UUT6	98	32	79	7.5	5.0	8.0

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.42	1.0	1.5	3.87	2.90	1.61	0.65

**Unit Mounting Description:**

The unit was base mounted to the shake table interface frame using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced approximately 30" widthwise and 95" lengthwise on center.



# UUT7

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSQ15064L5 (controller/pump skid)

**Product Construction Summary:** Powder coated structural steel skid and frame. Unit is internally isolated.

### Options / Component Summary:

5HP scroll pumps with WEG motors, dew point monitor, CO monitor, PBMI\_PXMI controller in NEMA 12 enclosure, timer drain, aftercooler, intake filter element and check valve.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
2,950	UUT7	108*	34	96*	4.5	4.0	4.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

\*Note: Length and height are combined dimensions for UUT7 and UUT5b.

### Unit Mounting Description:



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced approximately 32" widthwise and 95" lengthwise on center.

# UUT9

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** Desiccant air dryers NDL110 and NDL2110

**Product Construction Summary:**

Powder coated structural steel skid and frame

**Options / Component Summary:** NDL110 and NDL2110 desiccant air dryers.

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
800	UUT9	55.0	31.5	67.0	6.5	6.5	19.5

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**



The unit was base mounted to the shake table interface frame through the skid using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 30" widthwise and 53" lengthwise on center.

# UUT10a,b

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSD15B44K5 controller/pump skid (UUT10a) and receiver/dryer skid (UUT10b)

**Product Construction Summary:** Powder coated structural steel skid and frame. UUT10a is internally isolated.

**Options / Component Summary:** 7.5 HP scroll pumps with WEG motors, 120 gallon vertical receiver tank, CO monitor, BASIC\_PSM controller, aftercooler, intake filter element, PMD45 desiccant air dryer

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,550	UUT10a	61.0	33.0	78.0	6.5	4.5	24.0
840	UUT10b	61.0	34.0	76.0	4.0	6.0	23.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



Each skid was base mounted to the shake table interface frame with four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 30.5" widthwise and 57.5" lengthwise on center for both skids.



# UUT11ai,bi

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSQ20B62P5 controller/pump skid (UUT11ai) and receiver/dryer skid (UUT11bi)

**Product Construction Summary:** Powder coated structural steel skid and frame. UUT11ai is internally isolated.

**Options / Component Summary:** 10 HP scroll pumps with WEG motors, 240 gallon vertical receiver tank, CO monitor, PBMI\_PXMI controller, aftercooler, intake filter element, check valve, NDL130 desiccant air dryer

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.


### UUT Properties

Operating Weight (lb)		Dimensions (in)			Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
3,120	UUT11ai	79.0	34.0	78.0	3.0	3.0	7.5
1,680	UUT11bi	79.0	43.0	93.0	4.5	4.0	17.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	1.00	1.0	1.5	1.60	1.20	0.67	0.27

### Unit Mounting Description:

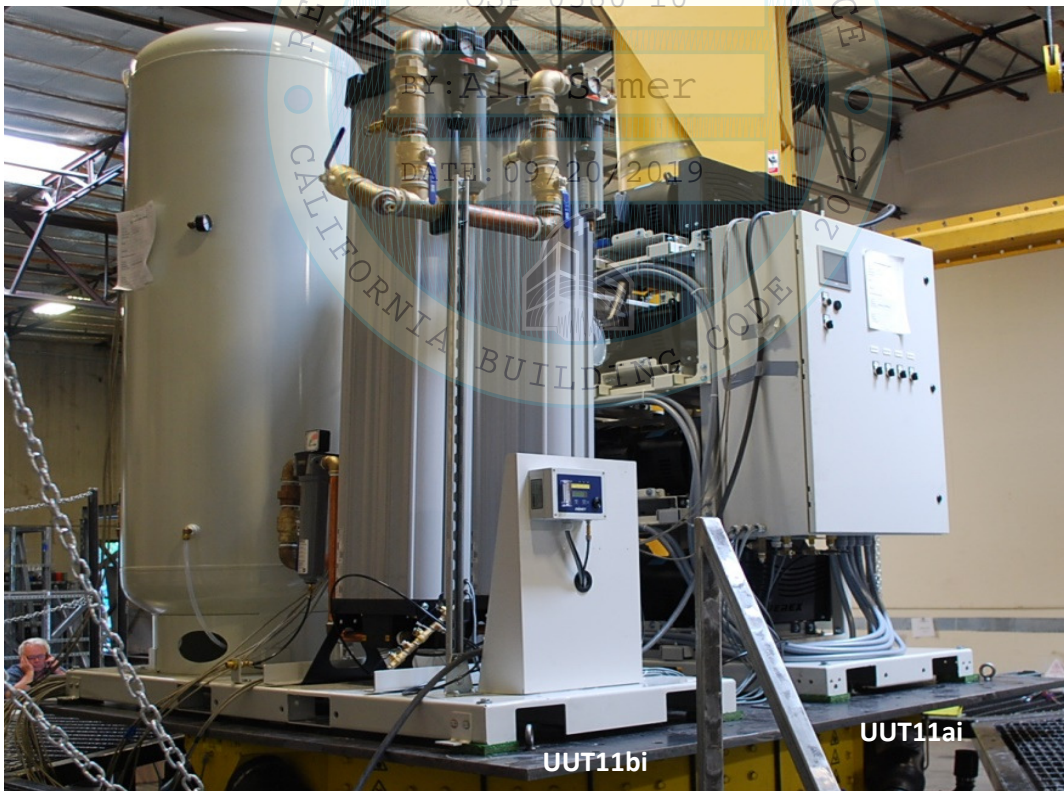

Each skid was base mounted to the shake table interface frame using four Airloc model 32 neoprene pads and four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 31' widthwise and 74" lengthwise on center for UUT 11ai and 42" widthwise and 74" lengthwise on center for UUT 11bi.



# UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSQ20B62P5 controller/pump skid (UUT11aii) and receiver/dryer skid (UUT11bii)

**Product Construction Summary:** Powder coated structural steel skid and frame. UUT11aii is internally isolated.

**Options / Component Summary:** 10 HP scroll pumps with WEG motors, 240 gallon vertical receiver tank, CO monitor, PBMI\_PXMI controller, aftercooler, intake filter element, check valve, NDL130 desiccant air dryer

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

## UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
3,120	UUT11aii	79.0	34.0	78.0	3.0	3.0	7.5
1,680	UUT11bii	79.0	43.0	93.0	4.5	4.0	17.0

## Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

## Unit Mounting Description:



Each skid was base mounted to the shake table interface frame with four 1/2"-diameter, Grade 5 bolts and washers spaced at approximately 31' widthwise and 74" lengthwise on center for UUT 11ai and 42" widthwise and 74" lengthwise on center for UUT 11bi.

# UUT12a

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MDRC05074FA5 (pump skid)

**Product Construction Summary:** Painted carbon steel enclosure. Unit is internally isolated.

**Options / Component Summary:** 50 HP pumps with WEG motors, aftercooler, intake filter element and check valve

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
2,930	UUT12a	77.5	39.4	65.2	5.5	6.0	28.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was base mounted with four 7/16"-diameter Grade 8 bolts and washers, and four 3"x3"x1/4" galvanized finish low carbon steel washers spaced approximately 38" widthwise and 34" lengthwise on center. Pre-test retrofit: the side panels were bolted to the enclosure frame with an additional four 5/16-inch diameter Grade 5 bolts, nuts, and washers each.

# UUT12b

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MDRC05074FA5 (dryer/controller skid)

**Product Construction Summary:** Powder coated structural steel skid and frame

**Options / Component Summary:** Quadruplex controller and NDL2120 and NDL4130 desiccant air dryers

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,760	UUT12b	32.0	99.2	80.3	5.0	10.5	>33.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



UUT12b Front View



UUT12b Side View

The unit was base mounted with four 1/2"-diameter Grade 5 bolts and washers spaced approximately 96" widthwise and 30" lengthwise on center., and four 3"x3"x3/16" galvanized finish low carbon steel washers.



# UUT12c

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MDRC05074FA5 (400 gallon receiver tank)

**Product Construction Summary:** Painted carbon steel

**Options / Component Summary:** 400 gallon vertical receiver tank

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
640	UUT12c	38.2	47.2	101.5	14.0	14.5	>33.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was base mounted with four 1/2"-diameter Grade 8 bolts spaced approximately 19" widthwise and 19" lengthwise on center, each with a 1/2" full size Grade 8 washer, 5/8" full size Grade 8 washer, and 2"x2"x3/16" low carbon steel black oxide finish plate washer.

# UUT14a

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSED200425 (pump skid)

**Product Construction Summary:** Painted carbon steel enclosure. Unit is internally isolated.

**Options / Component Summary:** 5 HP pumps with WEG motors, check valves

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,030	UUT14a	46.4	35.2	61.2	4.5	5.5	>33.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was base mounted with four 1/2"-diameter Grade 5 bolts and washers spaced approximately 28" widthwise and 33" lengthwise on center, and four 1 1/2"x1 1/2"x1/4" galvanized finish low carbon steel washers.

**UUT14b****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** MS200425 (controller skid); 2 controllers tested: PXEM218G2AJ and PXEM418G2AJ**Product Construction Summary:** Powder coated structural steel skid**Options / Component Summary:** Custom skid with duplex and quadruplex PXE controllers**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
560	UUT14b	55.0	39.8	79.4	11.0	9.5	>33.3

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**

UUT14b - duplex panel



UUT14b - quadruplex panel

The unit was base mounted with four 1/2"-diameter Grade 5 bolts and washers spaced approximately 30" widthwise and 52" lengthwise on center., and four 1 1/4"x1 1/4" x 3/8" malleable iron bevel washers, plain finish. Each control panel was braced to the skid with one piece of B-Line B45 14 gage galvanized carbon steel channel, attached with B-Line B230 brackets (one bracket per channel end) and two Grade 2, 1/2"-diameter bolts and nuts with flat washers per bracket.



# UUT15a

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** LSEQ60B845 (pump skid)

**Product Construction Summary:** Painted carbon steel enclosure. Unit is internally isolated.

**Options / Component Summary:** 10 HP pumps with WEG motors, check valves

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
2,740	UUT15a	51.0	73.8	61.2	5.0	6.0	>33.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was base mounted with four 1/2"-diameter Grade 5 bolts and washers spaced approximately 72" widthwise and 37" lengthwise on center, and four 1 1/2"x1 1/2"x1/4" galvanized finish low carbon steel washers. Pre-test retrofit: the top diaphragm corners were welded together, and the side panels were bolted to the frame with an additional four 5/16-inch diameter Grade 5 bolts, nuts and washers each.



# UUT15b

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** LSEQ60B845 (660 gallon receiver tank)

**Product Construction Summary:** Carbon steel

**Options / Component Summary:** 660 gallon vertical receiver tank

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,500	UUT15b	42.0	42.0	126.5	14.5	9.5	>33.3

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was base mounted with four 1/2"-diameter Grade 8 bolts and washers spaced approximately 20" widthwise and 20" lengthwise on center, and four 3"x3"x3/16" galvanized finish low carbon steel washers.

# UUT28

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Gas Automatic Changeover Manifolds

**Model Number:** PX-NPCU12A11L

**Product Construction Summary:** Powder coated carbon steel enclosure

**Options / Component Summary:** Regulators, circuit boards, power supply, transducers, switches, valves, gages and pipe adapters

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Depth	Width	Height	Front-Back	Side-Side	Vertical
66	UUT28	9.0	15.0	25.0	N/A	N/A	N/A

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was mounted to the shake table wall fixture with a combination of two manufacturer-provided channeled mounting brackets mounted near the top of the enclosure back plate, and two 3/8-inch diameter Grade 5 bolts spaced approximately 20" on center installed near the middle of the enclosure back plate. For the two mounting brackets, one was attached to the back plate of the cabinet with two 5/16-inch diameter Grade 5 bolts, and one was attached to the shake table interface frame with two 3/8-inch diameter Grade 5 bolts, and ¼-inch thick plate washers as a backing between the wall bracket and the shake table interface fixture.

The mounting locations were spaced 11" in the vertical direction.

# UUT29

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Gas Automatic Changeover Manifolds

**Model Number:** PX-LLU22NT3H

**Product Construction Summary:** Powder coated carbon steel enclosure

**Options / Component Summary:** Regulators, circuit boards, power supply, transducers, switches, valves, gages and pipe adapters

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Depth	Width	Height	Front-Back	Side-Side	Vertical
70	UUT29	11.0	19.0	27.0	N/A	N/A	N/A

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



The unit was mounted to the shake table wall fixture with a combination of two manufacturer-provided channeled mounting brackets mounted near the top of the enclosure back plate, and two 3/8-inch diameter Grade 5 bolts spaced approximately 20" on center installed near the middle of the enclosure back plate. For the two mounting brackets, one was attached to the back plate of the cabinet with two 5/16-inch diameter Grade 5 bolts, and one was attached to the shake table interface frame with two 3/8-inch diameter Grade 5 bolts, and ¼-inch thick plate washers as a backing between the wall bracket and the shake table interface fixture.

The mounting locations were spaced 11" in the vertical direction.

**UUT30a****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** VES07285 (80gal tank) , VES07072 (240gal tank)**Product Construction Summary:** Powder coated structural steel skid**Options / Component Summary:** Platform frame mounted tanks

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,010	UUT30a	33.5	60.0	94.0	4.0	5.5	31.5

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**

UUT 30a was base mounted with four 1/2" diameter Grade 5 bolts and washers spaced approximately 50" widthwise and 31" lengthwise on center.



**UUT30b****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** VES07285 (80gal tank) , VES07072 (240gal tank)**Product Construction Summary:** Powder coated structural steel skid**Options / Component Summary:** Platform frame mounted tanks

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,010	UUT30b	33.5	60.0	94.0	3.0	3.5	10.5

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**

UUT 30b was base mounted with four 1/2" diameter Grade 5 bolts and washers spaced approximately 50" widthwise and 31" lengthwise on center through an Airloc model 32 neoprene pad.

**UUT31a****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** VES07285 (80gal tank) , VES04767 (120gal tank)**Product Construction Summary:** Powder coated structural steel skid**Options / Component Summary:** Ladder frame mounted tanks

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
630	UUT31a	32	55	75	8.5	11.5	>33.3

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**

UUT 31a was base mounted with four 1/2" diameter Grade 5 bolts and washers spaced approximately 53" widthwise and 30" lengthwise on center and four 1 1/4"x1 1/4" x 3/8" malleable iron bevel washers.

**UUT31b****UNIT UNDER TEST (UUT) Summary Sheet****Manufacturer:** Powerex**Product Line:** Medical Air and Laboratory Air**Model Number:** VES07285 (80gal tank) , VES04767 (120gal tank)**Product Construction Summary:** Powder coated structural steel skid**Options / Component Summary:** Ladder frame mounted tanks

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

**UUT Properties**

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
630	UUT31b	32	55	75	8.0	9.5	16.0

**Seismic Test Parameters**

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

**Unit Mounting Description:**

UUT 31b was base mounted with four 1/2" diameter Grade 5 bolts and washers spaced approximately 53" widthwise and 30" lengthwise on center and four 1 1/4"x1 1/4" x 3/8" malleable iron bevel washers through an Airloc model 32 neoprene pad.



# UUT32

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSD02A3

**Product Construction Summary:** Powder coated structural steel skid

**Options / Component Summary:** Medical air and laboratory air unit with Trident PD204A desiccant dryer

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.

### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
1,060	UUT32	51	31	75	4.5	9.5	21.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:



UUT 32 was base mounted with four 1/2"-diameter Grade 5 bolts and washers spaced approximately 30" widthwise and 20" lengthwise on center.

# UUT33i,ii

## UNIT UNDER TEST (UUT) Summary Sheet

**Manufacturer:** Powerex

**Product Line:** Medical Air and Laboratory Air

**Model Number:** MSP15A6

**Product Construction Summary:** Powder coated structural steel skid

**Options / Component Summary:** Medical air and laboratory air unit with Trident PD213A desiccant dryer

**Note:** The UUT was operational before and after shaking and was full of operating content during the tests. The structural integrity of the component and attachment system and force-resisting systems was maintained.


### UUT Properties

Operating Weight (lb)	Dimensions (in)				Lowest Natural Frequency (Hz)		
		Length	Width	Height	Front-Back	Side-Side	Vertical
2,110	UUT33i	86	34	91	5.0	6.5	27.5
4,030	UUT33ii	86	34	80	5.5	4.0	22.0

### Seismic Test Parameters

Building Code	Test Criteria	Sds (g)	z/h	Ip	Aflx-H (g)	Arig-H (g)	Aflx-V (g)	Arig-V (g)
CBC 2016	ICC-ES AC156	2.00	1.0	1.5	3.20	2.40	1.33	0.53

### Unit Mounting Description:

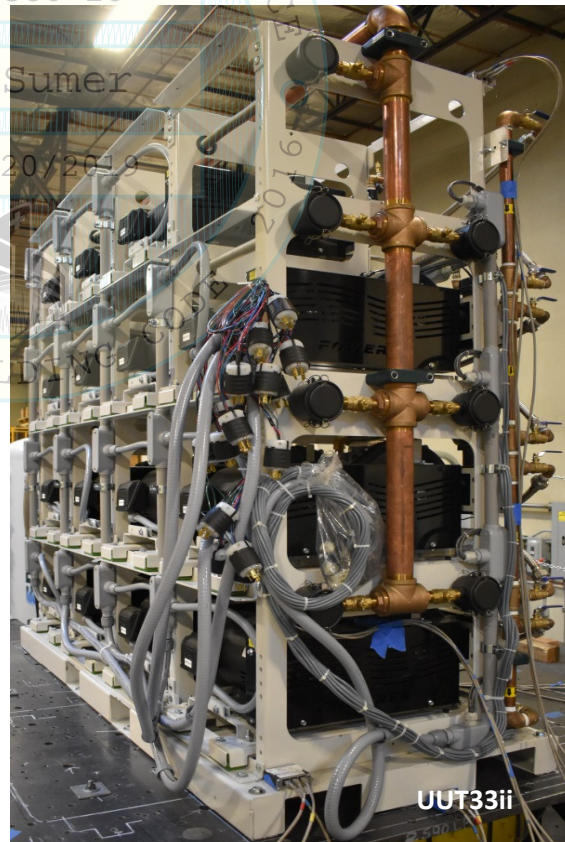

UUT 33i and 33ii was base mounted with eight 1/2"-diameter Grade 5 bolts and washers spaced approximately 31" widthwise and 20" lengthwise on center for both skids.